HIOKI

INSTRUCTION MANUAL

3561
3561-01

BATTERY HiTESTER

HIOKI E. E. CORPORATION

Contents

Introduction 1
Verifying Package Contents 1
Safety Information 2
Operating Precautions 4

Chapter 1 Overview 7

1.1 Product Overview 7
1.2 Features 8
1.3 Names and Functions of Parts 9
1.4 Menu Display Sequence (SHIFT → ENTER) 13
1.5 Measurement Flowchart 14

Chapter 2 Measurement Preparations 15

2.1 Preparation Flowchart 15
2.2 Connecting the Power Cord 16
2.3 Connecting the Optional Test Leads 17
2.4 Turning the Power On and Off 19
2.5 Selecting the Line Frequency 20

Chapter 3 Measurement 21

3.1 Pre-Operation Inspection 21
3.2 Basic Measurement Example 22
3.3 Selecting Measurement Mode 25
3.4 Setting Measurement Range 26
3.4.1 Manual Range Setting 26
3.4.2 Auto-Ranging 27
3.5 Setting Sampling Rate 28
3.6 Zero-Adjust Function 28
3.6.1 Wiring Method for Zero-Adjustment 28
3.6.2 Executing Zero-Adjustment 29
3.7 Displaying Measurement Results 31
3.7.1 Measurement Fault Detection 32
3.7.2 Overflow Display 32

Chapter 4
Applied Measurement ____ 33

4.1 Comparator Function 34
4.1.1 Comparator Setting Example 1 (Upper and Lower Threshold Judgment) 35
4.1.2 Comparator Setting Example 2 (Reference Value and Tolerance Judgment) 39
4.1.3 Comparator Judgment Beeper Setting 43
4.1.4 Comparator Execution Mode Setting 44
4.1.5 Comparator Threshold Method Selection 45
4.1.6 Upper and Lower Thresholds Setting (by Reference Value and Tolerance) 46
4.1.7 Enabling and Disabling the Comparator Function 48
4.1.8 Comparator Judgment Results 49
4.1.9 Switching Between Measurement Value and Comparator Setting Displays 50
4.2 Trigger Function 51
4.2.1 Trigger Source Settings 51
4.2.2 Trigger Delay Settings 52
4.3 Averaging Function 53
4.4 Statistical Calculation Functions 54
4.5 Memory Function 58
4.6 Key-Lock Function 60
4.7 Panel Save Function 61
4.8 Panel Load Function 62
4.9 Self-Calibration 63
4.10 Measurement Value Output Function 64
4.11 Key Beeper Setting 65
4.12 Reset Function 66

Chapter 5
External Control ____ 69

5.1 Overview 69
5.2 Signal Descriptions 70
5.2.1 Pinout 70
5.2.2 Input Signals 71
5.2.3 Output Signals 72
5.2.4 ERR Output 73
5.2.5 Instrument Settings 74
5.3 Timing Chart 75
5.4 Internal Circuitry 77

Chapter 6
Printer (Optional) 79

6.1 Connecting the Printer 80
6.1.1 Connecting the 9670 PRINTER to the Instrument 81
6.1.2 Loading Recording Paper 82
6.1.3 Charging the Battery Pack 83
6.1.4 Installing the Battery Pack in the Printer 83
6.2 Selecting the Interface 84
6.3 Setting of the 9670 PRINTER 84
6.4 Printing 85

Chapter 7
RS-232C/GP-IB Interfaces 87

7.1 Overview and Features 87
7.2 Specifications 88
7.2.1 RS-232C Specifications 88
7.2.2 GP-IB Specifications (Model 3561-01 only) 88
7.3 Selecting the Connections and Protocol 89
7.3.1 Attaching the Connector 89
7.3.2 Selecting the Interface 91
7.4 Communication Methods 92
7.4.1 Message Format 92
7.4.2 Output Queue and Input Buffer 97
7.4.3 Status Byte Register 98
7.4.4 Event Registers 100
7.4.5 Initialization Items 103
7.4.6 Local Function 103
7.5 Message List 104
7.5.1 Standard Commands 104
7.5.2 Device-Specific Commands 105
7.6 Message Reference 110
7.6.1 Standard Commands 111
7.6.2 Device-Specific Commands 115
7.6.3 Measurement Value Formats 141
7.6.4 Command Compatibility with the Model 3560 AC mΩ HiTESTER 142
7.7 Basic Data Importing Methods 146
7.8 Sample Programs 147

Chapter 8
Specifications 157

8.1 Basic Specifications 157
8.2 Accuracy 161
8.3 General Specifications 162

Chapter 9
Maintenance and Service 163

9.1 Troubleshooting 163
9.2 Cleaning 164
9.3 Error Display 164

Appendix 165

Appendix 1 Precautions for Making Custom Test Leads .. 165
Appendix 2 AC Four-terminal Method 167
Appendix 3 Synchronous Detection System 168
Appendix 4 Configuration and Extension of the Test Leads .. 169
Appendix 5 Effect of Eddy Currents 170
Appendix 6 Calibration Procedure 171
Appendix 7 Test Lead Options 172
Appendix 8 Rack Mounting 173
Appendix 9 Dimensional Diagram 175

Index i

Introduction

Thank you for purchasing the HIOKI "Model 3561, 3561-01 BATTERY HiTESTER." To obtain maximum performance from the instrument, please read this manual first, and keep it handy for future reference.

Verifying Package Contents

When you receive the instrument, inspect it carefully to ensure that no damage occurred during shipping. In particular, check the accessories, panel switches, and connectors. If damage is evident, or if it fails to operate according to the specifications, contact your dealer or Hioki representative.
Use the original packing materials when transporting the instrument, if possible.

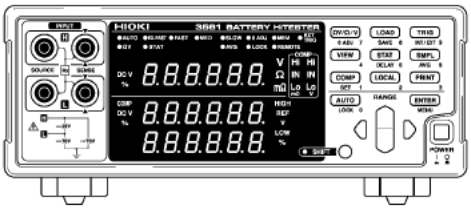

☐ Model 3561/ Model 3561-01 (GP-IB version)
BATTERY HiTESTER (1)



☐ Power cord (1)



☐ Instruction manual (this manual/ 1)

Options

☐ Model 9287-10	CLIP TYPE LEAD
☐ Model 9452	CLIP TYPE LEAD
☐ Model 9453	FOUR TERMINAL LEAD
☐ Model 9455	PIN TYPE LEAD (for ultra precision)
☐ Model 9467	LARGE CLIP TYPE LEAD
☐ Model 9770	PIN TYPE LEAD
☐ Model 9771	PIN TYPE LEAD
☐ Model 9637	RS-232C CABLE (9-pin to 9-pin/cross cable)
☐ Model 9638	RS-232C CABLE (9-pin to 25-pin/cross cable)
☐ Model 9151-02	GP-IB CONNECTOR CABLE (2 m)
☐ Model 9151-04	GP-IB CONNECTOR CABLE (4 m)
☐ Model 9670	PRINTER (BL-80RS II, made by SANEI ELECTRIC INC.)
☐ Model 9671	AC ADAPTER (for the 9670, BL-100W, made by SANEI ELECTRIC INC.)
☐ Model 9672	BATTERY PACK (for the 9670)
☐ Model 9673	BATTERY CHARGER (for the 9672)
☐ Model 9237	RECORDING PAPER (80 mm x 25 m, 4 rolls, for the 9670)

Safety Information

⚠WARNING

This instrument is designed to comply with IEC 61010 Safety Standards, and has been thoroughly tested for safety prior to shipment. However, mishandling during use could result in injury or death, as well as damage to the instrument. Be certain that you understand the instructions and precautions in the manual before use. We disclaim any responsibility for accidents or injuries not resulting directly from instrument defects.

This manual contains information and warnings essential for safe operation of the instrument and for maintaining it in safe operating condition. Before using it, be sure to carefully read the following safety precautions.

	In the manual, the symbol indicates particularly important information that the user should read before using the instrument. The symbol printed on the instrument indicates that the user should refer to a corresponding topic in the manual (marked with the ⚠ symbol) before using the relevant function.
	Indicates a grounding terminal.
	Indicates DC (Direct Current).
	Indicates AC (Alternating Current).
	Indicates the ON side of the power switch.
	Indicates the OFF side of the power switch.

The following symbols in this manual indicate the relative importance of cautions and warnings.

⚠DANGER	Indicates that incorrect operation presents an extreme hazard that could result in serious injury or death to the user.
⚠WARNING	Indicates that incorrect operation presents a significant hazard that could result in serious injury or death to the user.
⚠CAUTION	Indicates that incorrect operation presents a possibility of injury to the user or damage to the instrument.
NOTE	Indicates advisory items related to performance or correct operation of the instrument.

Other Symbols

	Indicates a prohibited action.
❖	Indicates the location of reference information.
	Indicates quick references for operation and remedies for troubleshooting.
*	Indicates that descriptive information is provided below.

Overvoltage Categories (CAT)

To ensure safe operation of measurement instruments, IEC 60664 establishes safety standards for various electrical environments, categorized as CAT I to CAT IV, and called overvoltage categories. These are defined as follows.

CAT I	Secondary electrical circuits connected to an AC electrical outlet through a transformer or similar device.
CAT II	Primary electrical circuits in equipment connected to an AC electrical outlet by a power cord (portable tools, household appliances, etc.)
CAT III	Primary electrical circuits of heavy equipment (fixed installations) connected directly to the distribution panel, and feeders from the distribution panel to outlets.
CAT IV	The circuit from the service drop to the service entrance, and to the power meter and primary overcurrent protection device (distribution panel).

Higher-numbered categories correspond to electrical environments with greater momentary energy. So a measurement device designed for CAT III environments can endure greater momentary energy than a device designed for CAT II.
Using a measurement instrument in an environment designated with a higher-numbered category than that for which the instrument is rated could result in a severe accident, and must be carefully avoided.

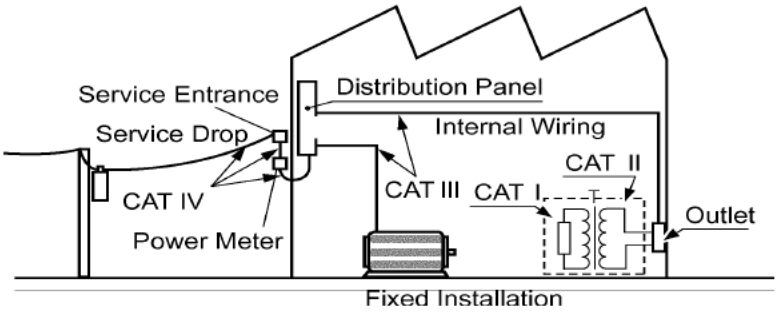

Accuracy

We define measurement tolerances in terms of f.s. (full scale), rdg. (reading) and dgt. (digit) values, with the following meanings:

f.s. (maximum display value or scale length)
The maximum displayable value or scale length. This is usually the name of the currently selected range.

rdg. (reading or displayed value)
The value currently being measured and indicated on the measuring instrument.

dgt. (resolution)
The smallest displayable unit on a digital measuring instrument, i.e., the input value that causes the digital display to show a "1" as the least-significant digit.

Operating Precautions

Follow these precautions to ensure safe operation and to obtain the full benefits of the various functions.

Instrument Installation and Operating Environment

Operating temperature and humidity:
0 to 40°C (32 ± 104°F), 80%RH or less (non-condensating)
Temperature and humidity range for guaranteed accuracy:
23 ± 5°C (73 ± 9°F), 80% RH or less (non-condensating)

Avoid the following locations that could cause an accident or damage to the instrument.

Exposed to direct sunlight
Exposed to high temperature

In the presence of corrosive or explosive gases

Exposed to liquids
Exposed to high humidity or condensation

Exposed to strong electromagnetic fields
Near electromagnetic radiators

Exposed to high levels of particulate dust

Subject to vibration

NOTE

Avoid using near electrically noisy devices, as the noise may impinge upon the test object and cause unreliable measurements.

Installation

Do not install the instrument with any side except the bottom facing down.

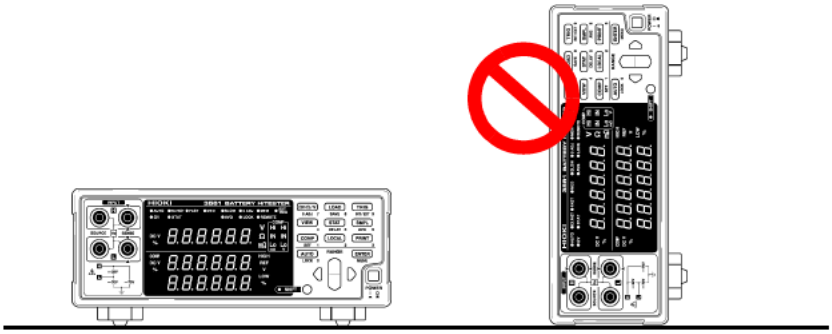

Preliminary Checks

Before using the instrument the first time, verify that it operates normally to ensure that the no damage occurred during storage or shipping. If you find any damage, contact your dealer or Hioki representative.

⚠WARNING

Before using the instrument, make sure that the insulation on the power cord and test leads is undamaged and that no bare conductors are improperly exposed. Using the instrument in such conditions could cause an electric shock, so contact your dealer or Hioki representative for replacements.

Measurement Precautions

⚠DANGER

- **To avoid electrical shock, be careful to avoid shorting live lines with the test leads.**
- **The maximum rated voltage between input terminals and ground is ± 70 V DC. Attempting to measure voltages exceeding 70 V with respect to ground could damage the instrument and result in personal injury.**

⚠WARNING

To avoid injury or damage to the instrument, do not attempt to measure AC voltage and AC current, or DC voltage exceeding ± 22 V.

NOTE

- Use only the specified test leads and cables. Using a non-specified cable may result in incorrect measurements due to poor connection or other reasons.
- To ensure certified measurement accuracy, allow at least 30 minutes warm-up. After warm-up, be sure to execute self-calibration.
  ❖See Section 4.9 Self-Calibration (Page 63).
- The input circuitry includes a protective fuse. Measurement is not possible when the fuse is blown.
- This instrument internally stores (backs up) all settings (except memory function and measurement values), such as measurement range, comparator settings and etc., but only when no operation is performed for a certain time. Therefore, to preserve settings, do not turn the power off for a short time (about five seconds) after changing a setting. However, measurement settings made through the RS-232C or GP-IB interface and measurement settings loaded by $\overline{\text{LOAD}}$ signals of the EXT I/O connector are not memorized.

Before Connecting and Powering On

⚠WARNING

- **Before turning the instrument on, make sure the supply voltage matches that indicated on the its power connector. Connection to an improper supply voltage may damage the instrument and present an electrical hazard.**
- **To avoid electrical accidents and to maintain the safety specifications of this instrument, connect the power cord only to a 3-contact (two-conductor + ground) outlet.**

NOTE

To suppress noise, the instrument needs to be set to match the frequency of the power source. Before operating, set the instrument to the frequency of your commercial power. If the supply frequency is not set properly, measurements will be unstable.
❖ See Section 2.5 Selecting the Line Frequency (Page 20).
Make sure the power is turned off before connecting or disconnecting the power cord.

Handling the Instrument

⚠WARNING

- **Never modify the instrument. Only Hioki service engineers should disassemble or repair the instrument. Failure to observe these precautions may result in fire, electric shock, or injury.**
- **The GP-IB connector location is covered by a blank panel on the Model 3561. To avoid electric shock, do not remove the blank panel.**

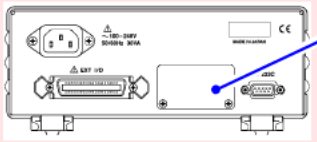

* This model is the 3561 BATTERY HiTESTER.

⚠CAUTION

- To avoid damage to the instrument, protect it from physical shock when transporting and handling. Be especially careful to avoid physical shock from dropping.
- Do not apply heavy downward pressure with the stand extended. The stand could be damaged.

Handling the Test Leads and Cables

⚠CAUTION

- To avoid breaking the test leads and cables, do not bend or pull them.
- Avoid stepping on or pinching cables, which could damage the cable insulation.

Chapter 1 Overview

1.1 Product Overview

The Model 3561 and 3561-01 BATTERY HiTESTERs measure battery internal resistance using a four-terminal, 1-kHz AC method, while simultaneously measuring DC voltage (electromotive force [emf]). The high-precision, fast measurement performance and extensive interface capabilities make these models ideal for incorporating into battery testing production lines.

1.2 Features

Simultaneously Measures Battery Internal Resistance and Voltage

The four-terminal AC method measures resistance and DC voltage simultaneously, so battery internal resistance and emf are measured and judged at once.

High-Precision Measurements

The instrument provides high-resolution resistance (0.01 mΩ) and voltage measurements (0.1 mV). High precision (± 0.01% rdg.) ensures accurate voltage measurements.

High-Speed Measurements

Simultaneous resistance and voltage measurements can be performed as fast as once every 10 ms.

Comparator Functions

Resistance and voltage measurement values are judged in three categories (Hi, IN and Lo), with results clearly displayed. A comparator judgment beeper also provides distinct sounds to indicate pass/fail judgments and to facilitate correct recognition of judgment results.

Statistical Calculation Functions

Maximum, minimum and average measurement values, standard deviation, process capability indices and other values can be automatically calculated for applications such as production management. Calculation results can also be applied as comparator setting values.

Measurement Value Memory Function

The instrument includes a Memory function and storage capacity for up to 400 pairs of measurement values. When making many sequential measurements at high speed and sending the measured values to a PC after each measurement, the time to switch test objects can become unsatisfactorily long. The Memory function can avoid the slow-down by sending stored measurements in batches during idle times.

EXT I/O Interface

EXT I/O and RS-232C interfaces are equipped as standard, supporting transfer rates up to 38,400 bps. Model 3561-01 also supports GP-IB.

Printing Measurement Values and Statistical Results

Connect the optional Model 9670 PRINTER to print measurement values and statistical calculation results.

1.3 Names and Functions of Parts

Front Panel

Input Terminals (INPUT)
Connect the optional test leads.
❖Connections:
See Section 2.3 Connecting the Optional Test Leads (Page 17).

Main Display
❖(Page 10)

Operating Keys
❖(Page 11)

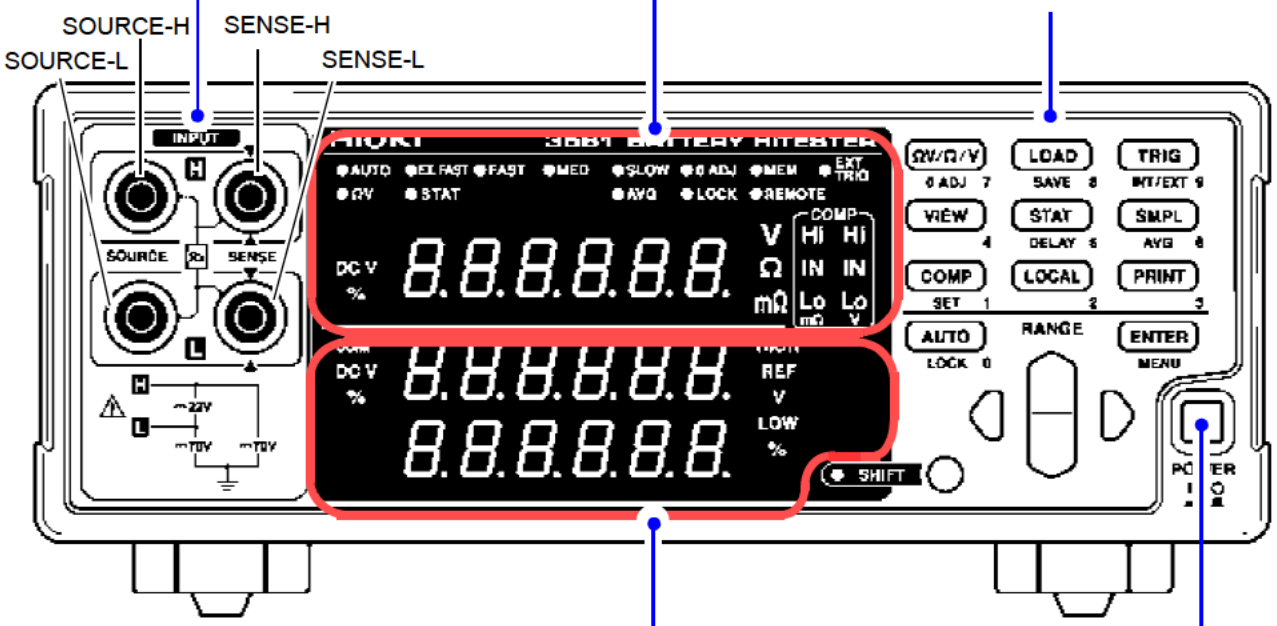

Sub Display
❖(Page 10)

POWER Switch
Turns the instrument on and off.
○ : Power OFF
| : Power ON
❖See Section 2.4 Turning the Power On and Off (Page 19).

Main Display

The current measurement mode is indicated while measuring, and the setting item is displayed while making settings.

(Upper row)

AUTO	Lit when measuring with Auto-Ranging.
EX.FAST, FAST, MED, SLOW	The selected Sampling Rate is lit.
0 ADJ	Lit when measuring in a range for which Zero-Adjustment has been performed.
MEM	Lit when the Memory function is enabled.
EXT TRIG	Lit when the External Trigger function is enabled.

(Lower row)

ΩV	Lit when the ΩV (Resistance and Voltage measurement) mode is selected.
STAT	Lit when the Statistical Calculation function is enabled.
AVG	Lit when measuring with the Averaging setting enabled.
LOCK	Lit when the keys are locked.
REMOTE	Lit during communications.

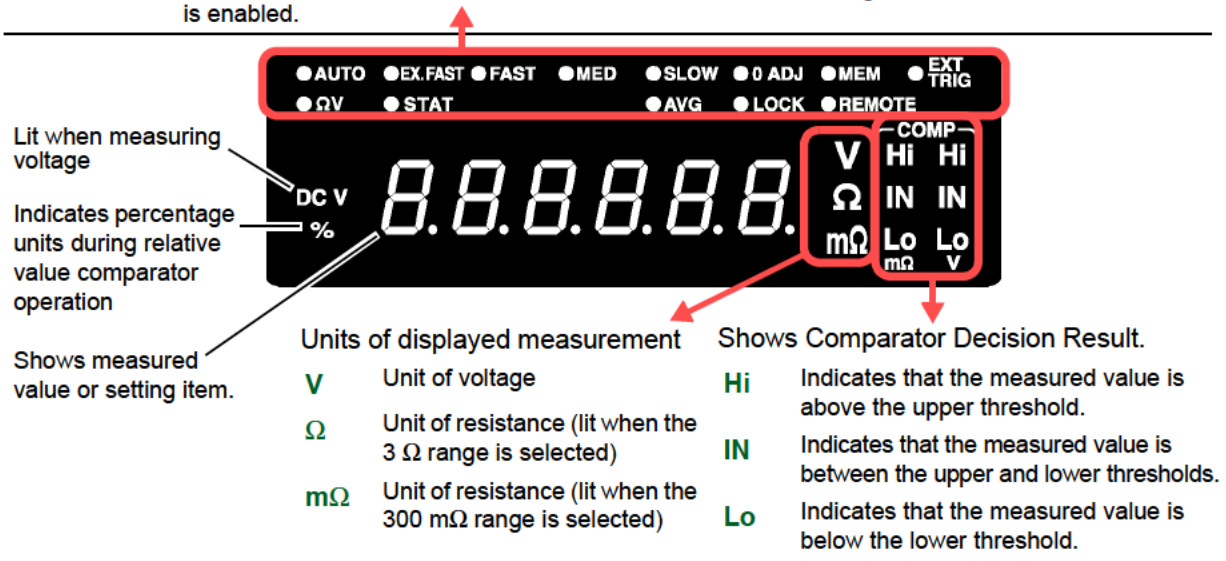

Units of displayed measurement

V	Unit of voltage
Ω	Unit of resistance (lit when the 3 Ω range is selected)
mΩ	Unit of resistance (lit when the 300 mΩ range is selected)

Shows Comparator Decision Result.

Hi	Indicates that the measured value is above the upper threshold.
IN	Indicates that the measured value is between the upper and lower thresholds.
Lo	Indicates that the measured value is below the lower threshold.

Sub Display

Upper and lower thresholds and other settings are displayed (when set).

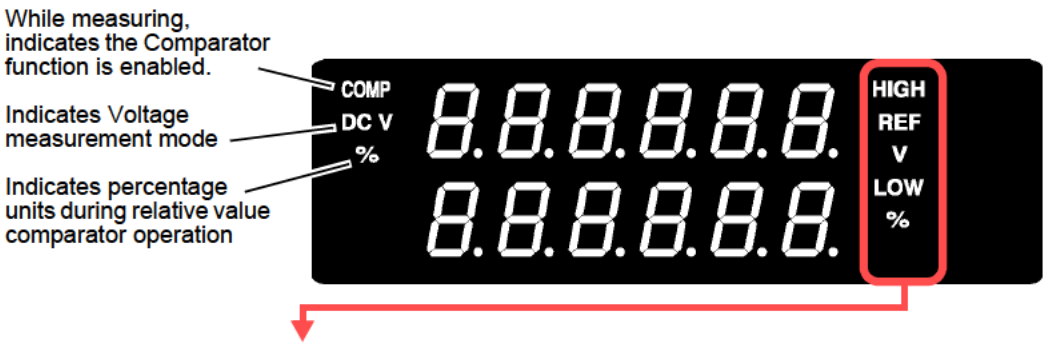

HIGH, LOW	Indicates that absolute value comparator operation is enabled (while measuring), and also when setting.
REF, %	Indicates that relative value comparator operation is enabled (while measuring), and also when setting.
V	Indicates voltage measurement units.

Operating Keys

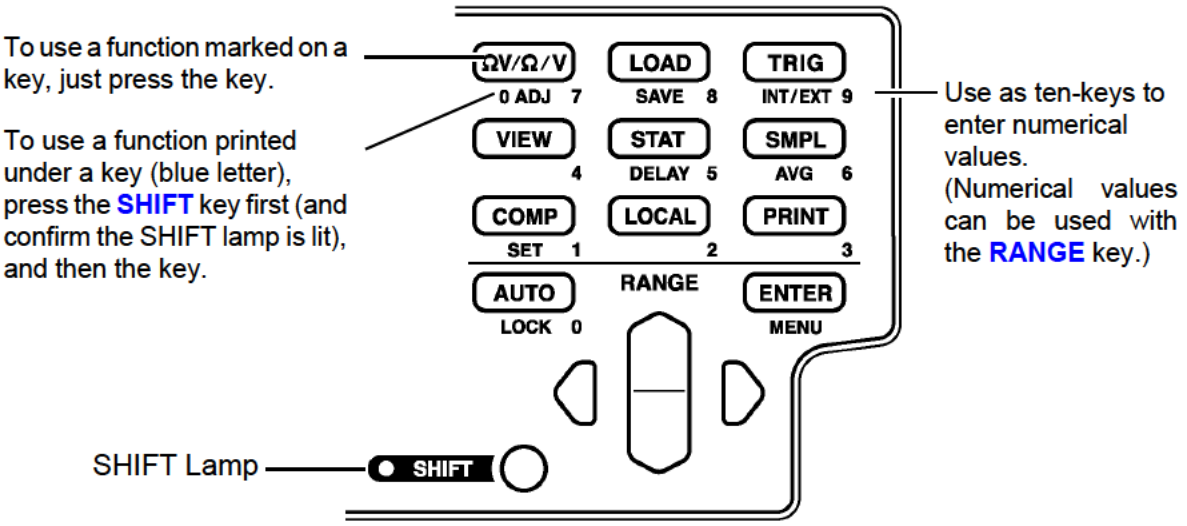

[ ]: Enabled after pressing the **SHIFT** key (SHIFT lamp lit).

Operating Key	Description
ΩV/ Ω/ V	Selects Measurement mode. (Resistance and voltage measurement, Resistance measurement or Voltage measurement)
[0 ADJ]	Executes Zero-Adjustment.
LOAD	Loads a saved measurement configuration (Panel settings).
[SAVE]	Saves the current measurement configuration (Panel settings).
TRIG	Executes a Manual Trigger event.
[INT/EXT]	Selects internal/external triggering.
VIEW	Switches the view mode of the ΩV mode.
STAT	Displays and sets Statistical Calculation results.
[DELAY]	Sets the Trigger Delay.
SMPL	Selects the Sampling Rate.
[AVG]	Activates Averaging function settings.
COMP	Switches the Comparator function on and off.
[SET]	Activates Comparator function setting.
LOCAL	Cancels remote control (RMT) and re-enables key operations.

Operating Key	Description
PRINT	Sends measurement values and statistical calculation results to the printer.
AUTO	Switches between Auto and Manual range selection.
[LOCK]	Switches the Key-Lock function on and off.
ENTER	Applies settings.
[MENU]	Selects various operating functions and settings.
RANGE	Up/Down: Changes setting value or numerical value, and range selection. Left/Right: Moves the setting item or digit.
SHIFT	• Enables the functions of the operating keys marked in blue. The lamp is lit when the SHIFT state is active. • Cancels settings in various setting displays. (Returns to the Measurement display without applying settings.) However, this does not apply to Menu display. However, from a menu item display, changed settings are not canceled, but accepted as the display returns to measurement display (except after Zero-Adjustment clear or resetting).

Rear Panel

Power Inlet
Connect the supplied power cord here.
❖See Section 2.2 Connecting the Power Cord (Page 16).

RS-232C Connector
Connection for the printer or RS-232C interface.
❖See Section 7.3.1 Attaching the Connector (Page 89).

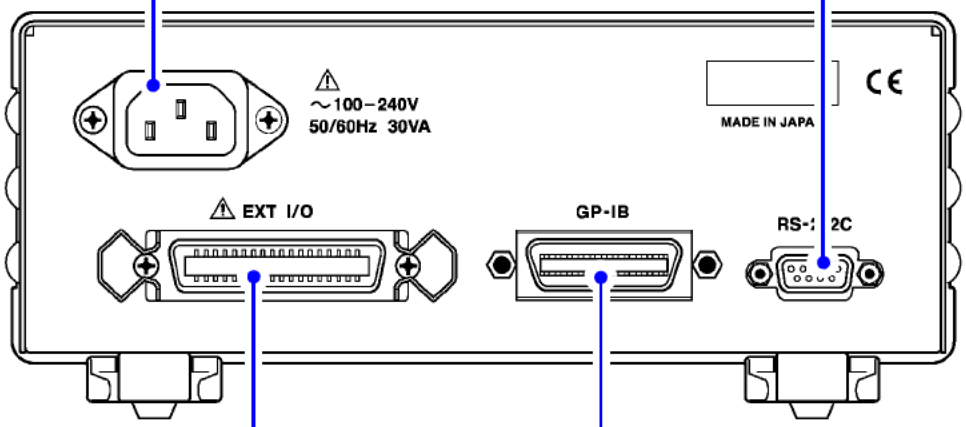

EXT I/O Connector
Connect here to use the EXT I/O interface.

GP-IB Connector (Model 3561-01 only)
Connect here to use the GP-IB interface.
❖7.3.1 Attaching the Connector (Page 89).

* The illustration shows the Model 3561-01 BATTERY HiTESTER (GP-IB version).

⚠WARNING

The GP-IB connector location is covered by a blank panel on the Model 3561. To avoid electric shock, do not remove the blank panel.

Side View

Stand
Can be opened to tilt the front panel upwards.

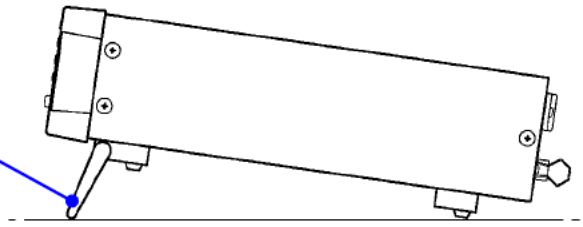

⚠CAUTION

Do not apply heavy downward pressure with the stand extended. The stand could be damaged.

1.4 Menu Display Sequence (SHIFT → ENTER)

Various auxiliary settings can be performed from the menu item displays.

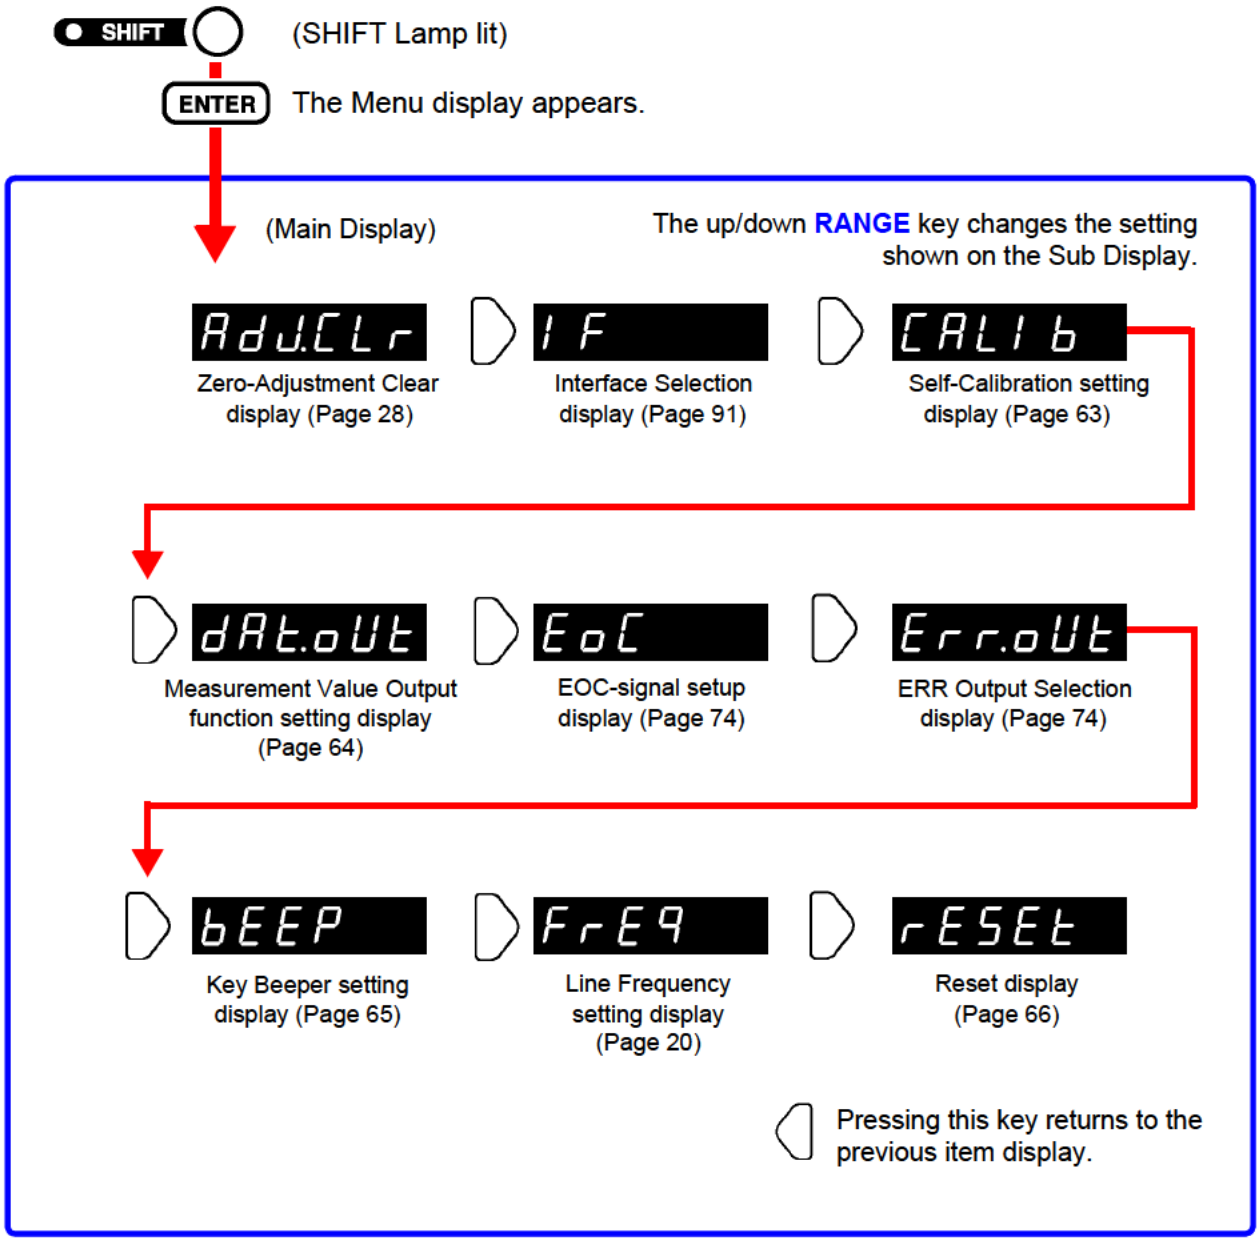

NOTE Settings on the menu item displays are applied and saved internally when changed.

1.5 Measurement Flowchart

The basic measurement process flow is as follows:

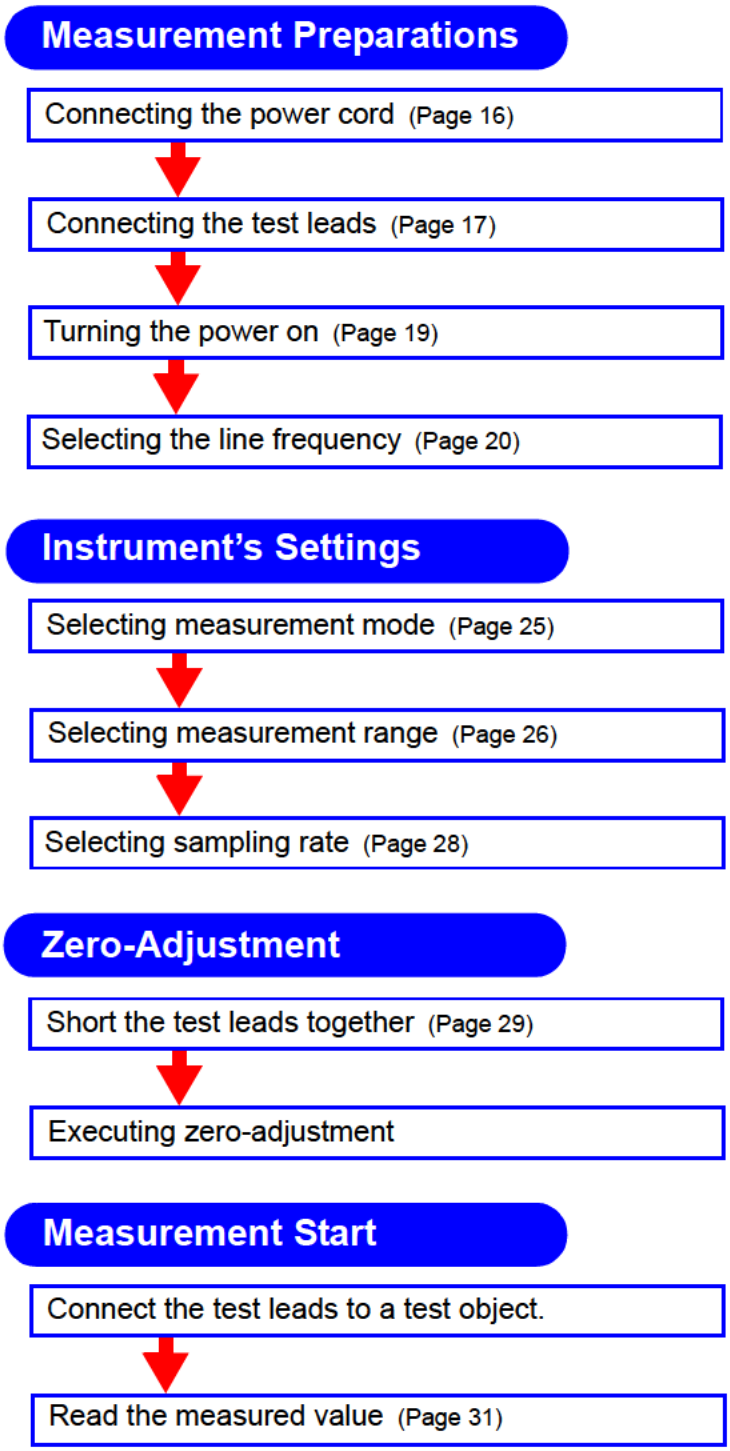

For details about the functions that can be applied to measurement values such as comparator, trigger and averaging functions, refer to Chapter 4 Applied Measurement (Page 33).

Measurement Preparations Chapter 2

2.1 Preparation Flowchart

This procedure describes instrument preparations such as making connections and turning power on.

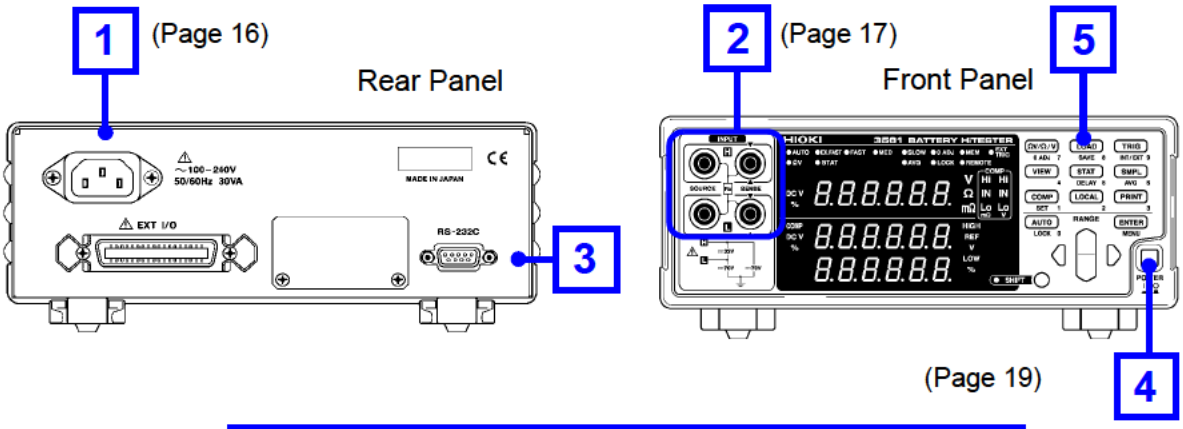

1 Connecting the power cord. (Page 16)

↓

2 Connect the test leads to the instrument. (Page 17)

↓

3 Connect the EXT I/O connector and interface connector. (Page 89)

↓

4 Turn the power on. (Page 19)

↓

5 Set measurement settings. (Page 21)

↓

6 Start measurement.

NOTE

Verify that the instrument's line frequency is correctly set when using it for the first time and after initialization following repair or recalibration.

❖See Section 2.5 Selecting the Line Frequency (page 20).

2.2 Connecting the Power Cord

⚠WARNING

To avoid electrical accidents and to maintain the safety specifications of this instrument, connect the power cord only to a 3-contact (two-conductor + ground) outlet.

⚠CAUTION

To avoid damaging the power cord, grasp the plug, not the cord, when unplugging it from the power outlet.

NOTE

To suppress noise, the instrument needs to be set to match the line frequency.
Before operating, set the instrument to the frequency of your commercial power. If the supply frequency is not set properly, measurements will be unstable.
❖ See Section 2.5 Selecting the Line Frequency (page 20).
Make sure the power is turned off before connecting or disconnecting the power cord.

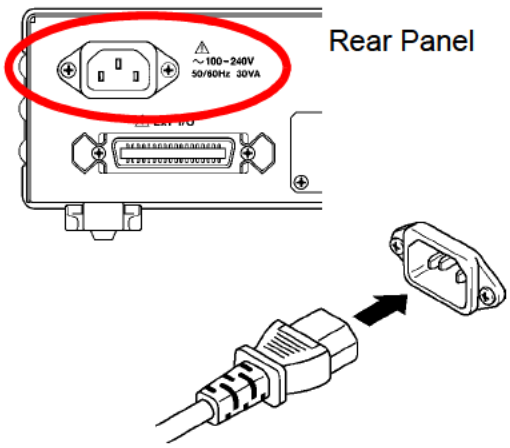

Rear Panel

1. **Confirm that the instrument's Power switch is OFF.**
2. **Check that the power supply voltage is correct, and connect the power cord to the power inlet socket on the rear of the instrument.**
3. **Plug the power cord into the AC outlet.**

2.3 Connecting the Optional Test Leads

Test leads are not included as standard accessories with the instrument, so the appropriate options need to be purchased separately or constructed according to the user's application requirements. To construct custom test leads, refer to Appendix 1 Precautions for Making Custom Test Leads (page 165). The resistance measurement terminals on this instrument consist of four separate banana jacks.

❖See Appendix 1 Precautions for Making Custom Test Leads (page 165).

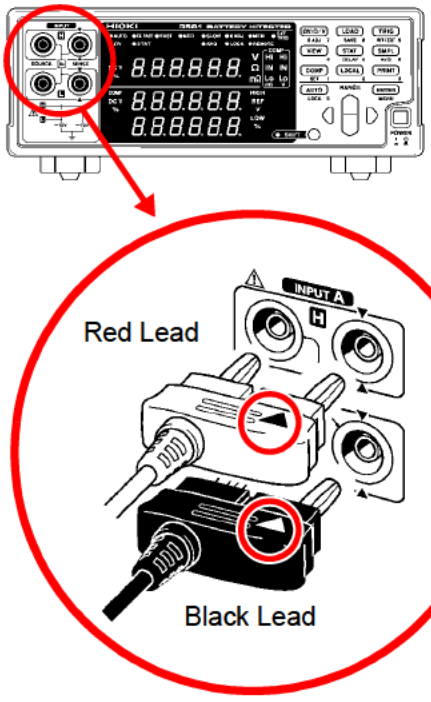

1. **Confirm that the instrument's Power switch is OFF.**

2. **Connect four-terminal test leads such as the 9287-10 CLIP TYPE LEAD to INPUT A.**

Plug the ▲ mark on the red lead into the red ▲ marked jack on the instrument,
and plug the ▲ mark on the black lead into the black ▲ marked jack on the instrument.

Example: Optional model 9287-10 CLIP TYPE LEAD

About Test Leads

(Example: Model 9287-10 CLIP TYPE LEAD)

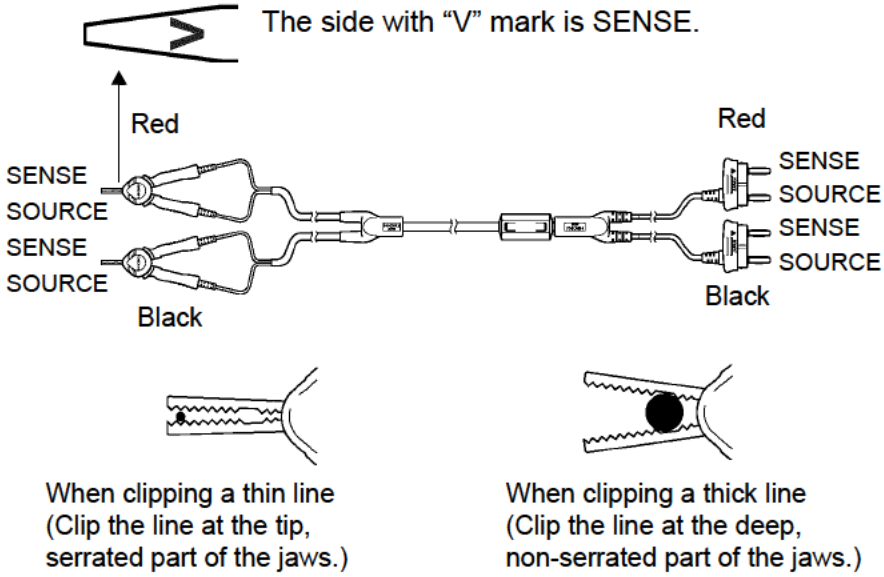

When clipping a thin line
(Clip the line at the tip,
serrated part of the jaws.)

When clipping a thick line
(Clip the line at the deep,
non-serrated part of the jaws.)

2.4 Turning the Power On and Off

⚠WARNING

Before turning the instrument on, make sure the supply voltage matches that indicated on the its power connector. Connection to an improper supply voltage may damage the instrument and present an electrical hazard.

NOTE

- The measurement setting state is the same as when the power was previously turned off (backup).
  To preserve changes to settings, wait a short time (about five seconds) after changing a setting before turning power off.
- However, measurement settings made through the RS-232C or GP-IB interface and measurement settings loaded by LOAD signals of the EXT I/O connector are not memorized.
- Before starting to measure, allow 30 minutes for warm-up.
  After warm-up, be sure to perform a self-calibration.
  ❖ See Section 4.9 Self-Calibration (page 63).

Turning the Power On

Power ON |

Turn the POWER switch ON (|).

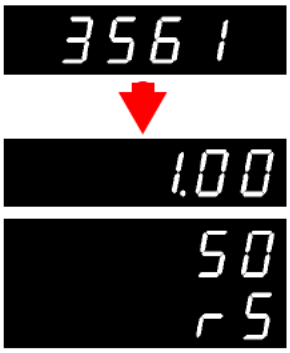

(Main Display)
Model name

(Main Display)
Software version

(Sub Display)
Line frequency

Interface

The measurement display appears.

Turning the Power Off

Power OFF ○

Turn the POWER switch OFF(○).

2.5 Selecting the Line Frequency

Verify that the instrument's line frequency is correctly set when using it for the first time and after initialization following repair or recalibration.

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

(Main Display)

(Sub Display)

2

Select the Line Frequency setting display.

❖ See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (page 13).

(Main Display)

(Sub Display) flashing

3

Select the frequency of the AC mains supply being used.

(Main Display)

(Sub Display) flashing

50..... 50 Hz
60..... 60 Hz

4 ENTER

Applies settings and returns to the Measurement display.

NOTE

To suppress noise, the instrument needs to be set to match the frequency of the power source.
Before operating, set the instrument to the frequency of your commercial power. If the supply frequency is not set properly, measurements will be unstable.

Chapter 3 Measurement

Before starting measurement, please read Operating Precautions (Page 4) and Chapter 2 Measurement Preparations (Page 15).

DANGER

- **To avoid electrical shock, be careful to avoid shorting live lines with the test leads.**
- **The maximum rated voltage between input terminals and ground is ± 70 V DC. Attempting to measure voltages exceeding 70 V with respect to ground could damage the instrument and result in personal injury.**

WARNING

To avoid injury or damage to the instrument, do not attempt to measure AC voltage and AC current, or DC voltage exceeding ± 22 V.

3.1 Pre-Operation Inspection

Before using the instrument, perform the following inspection to ensure that it is operating properly.

Check Point	Check Contents
Instrument Chassis (both front and rear panels)	• No damage or cracks • No internal circuitry is exposed
Test Leads and Power Cord	• Metal parts that should be insulated are not exposed
Good Test Sample	• Measures as good and displays the correct measurement value
Bad Test Sample	• Measures as bad and displays the correct measurement value

If the inspection reveals a defect, stop using the instrument and contact your dealer or Hioki representative.

3.2 Basic Measurement Example

The following example describes the measurement process.

Example: Measuring resistance and voltage of a 30 mΩ lithium-ion battery

Required items:	Lithium-ion battery (30 mΩ) Test leads: Model 9770 PIN TYPE LEAD are used here.
Measurement conditions:	Measurement mode ..... ΩV (Resistance and Voltage measurement) Range ..... 300 mΩ Sampling rage..... SLOW Zero adjustment ..... Enabled

Preparations

1 **Connect the power cord.**

❖See Section 2.2 Connecting the Power Cord (Page 16).

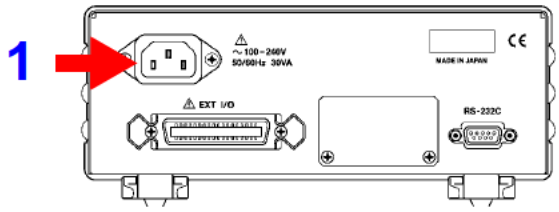

2 **Connect the test leads.**

❖See Section 2.3 Connecting the Optional Test Leads (Page 17).

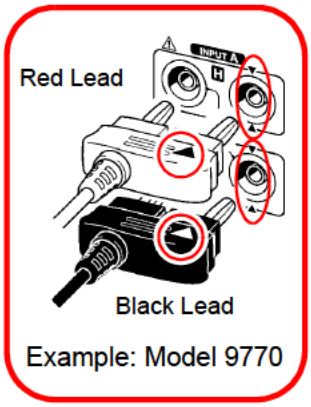

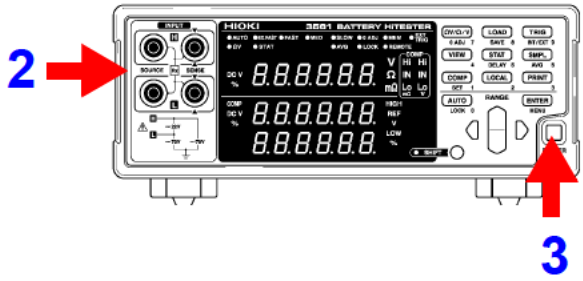

3 **Turn the power on.**

❖See Section 2.4 Turning the Power On and Off (Page 19).
❖See Section 2.5 Selecting the Line Frequency (Page 20).

Instrument Settings

4 **Confirm the SHIFT lamp is not lit.**
If this is lit, press the **SHIFT** key to turn it off.

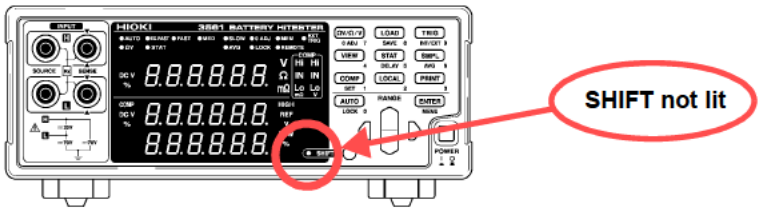

5 ΩV/Ω/V **Select the Resistance Measurement mode.**
(Here, resistance and voltage measurement is selected.)
❖See Section 3.3 Selecting Measurement Mode (Page 25).

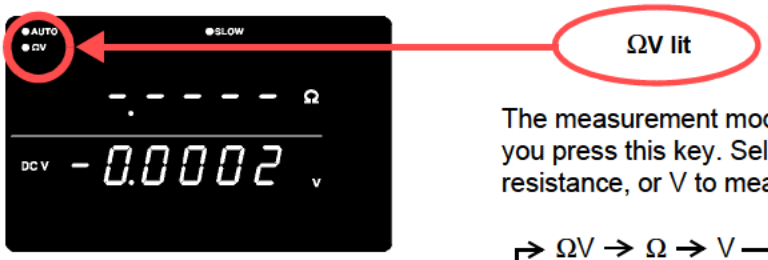

The measurement mode changes each time you press this key. Select Ω to measure only resistance, or V to measure only voltage.

→ ΩV → Ω → V →

6 **Set the measurement range.** (Here, 300 mΩ range is selected.)
❖See Section 3.4 Setting Measurement Range (Page 26).

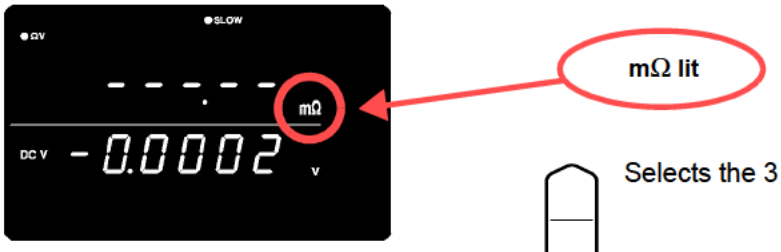

Selects the 3 Ω range (Ω lit)

Selects the 300 mΩ range (mΩ lit)

7 SMPL **Set the sampling rate.** (Here, SLOW is selected.)
❖See Section 3.5 Setting Sampling Rate (Page 28).

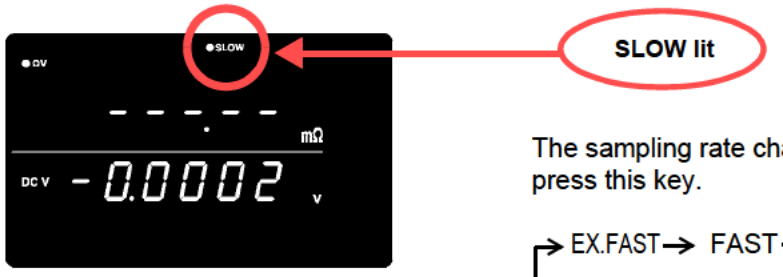

The sampling rate changes each time you press this key.

→ EX.FAST → FAST → MED → SLOW →

Zero-Adjustment

8 **Short the test leads together.**
Proper Zero-Adjustment is not possible with incorrect wiring.

❖See Section 3.6 Zero-Adjust Function (Page 28).

Example: Model 9770 PIN TYPE LEAD

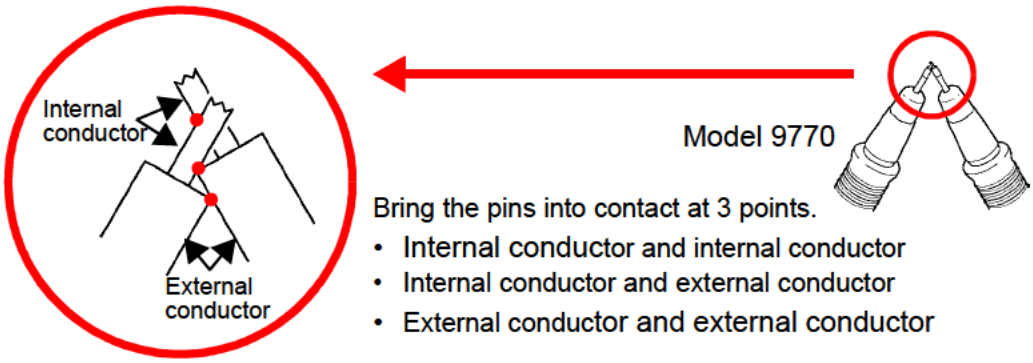

Bring the pins into contact at 3 points.
- Internal conductor and internal conductor
- Internal conductor and external conductor
- External conductor and external conductor

9 SHIFT ○ **(SHIFT Lamp lit)**

ΩV/Ω/V
0 ADJ

Execute Zero-Adjust.
After zero-adjustment, the display returns to the measurement mode.

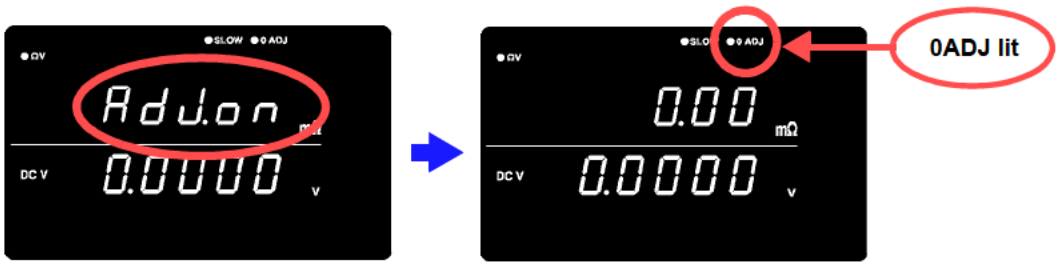

"Err.02" appears if Zero-Adjustment fails. Verify that the test lead tips are properly shorted, and try zero-adjustment again.

Measurement

10 **Connect the test leads to a battery.**



11 **Read the measured resistance and voltage.**

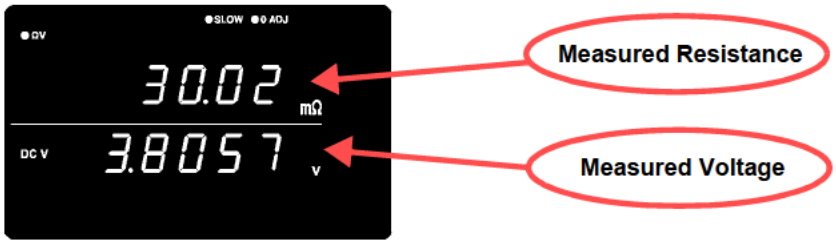

❖See Section 3.7 Displaying Measurement Results (Page 31).
❖See Section 9.3 Error Display (Page 164).

3.3 Selecting Measurement Mode

Select the measurement mode from ΩV (both resistance and voltage measurement), Ω (resistance measurement only) or V (voltage measurement only).

1

Confirm the SHIFT lamp is not lit.
If this is lit, press the **SHIFT** key to turn it off.

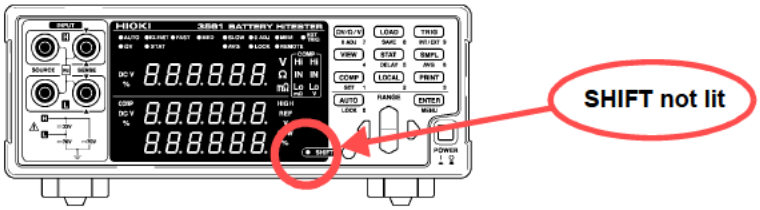

2 [ΩV/Ω/V]

Switches the displayed measurement mode.
Each key-press switches the measurement mode.

ΩV mode
(Resistance and Voltage measurement)

"ΩV" indicates the ΩV mode is selected

"Ω" indicates the 3 Ω range is selected
"mΩ" indicates the 300 mΩ range is selected

Ω mode
(Resistance measurement)

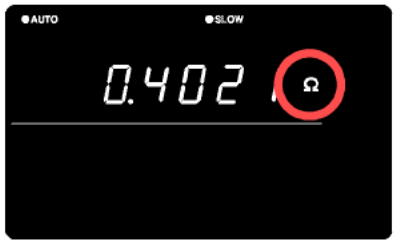

V mode
(Voltage measurement)

[ΩV/Ω/V]

NOTE

The fastest measurements are provided by selecting the Ω or V mode when measuring resistance or voltage, respectively.
❖See Section Sampling Time (Page 158).

3.4 Setting Measurement Range

Select the resistance measurement range from 3 Ω (“Ω” indicator lit) or 300 mΩ (“mΩ” indicator lit). The auto-ranging function can be enabled to automatically determine the most suitable range. The voltage measurement range is fixed at 20 V.

3.4.1 Manual Range Setting

1

When auto-ranging is enabled, pressing this disables it (AUTO not lit) and enables manual range selection.

2 **Select the range to use.**

When the 3 Ω range is selected

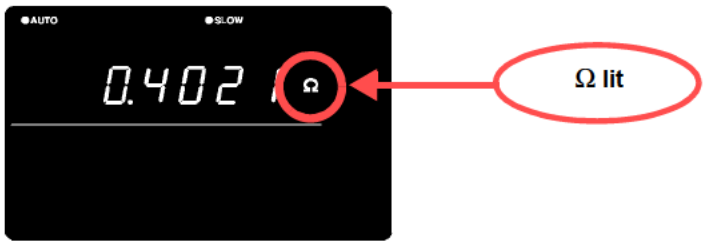



3 Ω range

When the 300 mΩ range is selected

300 mΩ range

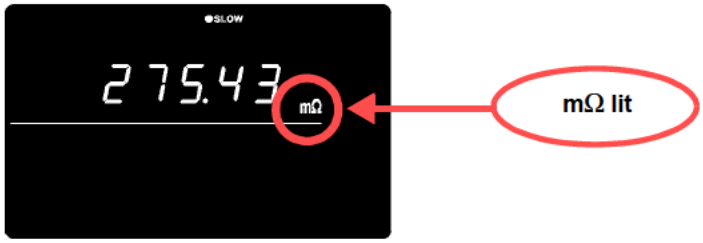

3.4.2 Auto-Ranging

AUTO

When manual range selection is enabled, pressing this enables **auto-ranging**. The most suitable measurement range is then selected automatically.

Switching from Auto-ranging back to Manual range selection

Press the **AUTO** key again. The range can now be changed manually.

NOTE

- Voltage measurement has only one range. The range cannot be changed.
- Depending on the state of the test object, auto-ranging may be unstable. In this case, select the range manually, or increase the Delay time.
  ❖See Section 3.4.1 Manual Range Setting (Page 26).
- Auto-ranging is not available when Comparator or Memory functions are enabled (ON).
- Refer to Chapter 8 Specifications (Page 157) for details about accuracy.

Range	Displayed Values	Resistance Measurement Mode	
		Measured Current	Open-Terminal Voltage
300 mΩ	-10.00 to 310.00 mΩ	10 mA ± 10%	7 Vpeak.
3 Ω	-0.1000 to 3.1000 Ω	1 mA ± 10%	7 Vpeak.
20 V	-19.9999 to 19.9999 V	--	7 Vpeak.

3.5 Setting Sampling Rate

The sampling rate can be selected from EX.FAST, FAST, MEDIUM and SLOW. Slower sampling rates generally provide greater measurement precision.

SMPL **Selects the sampling rate**

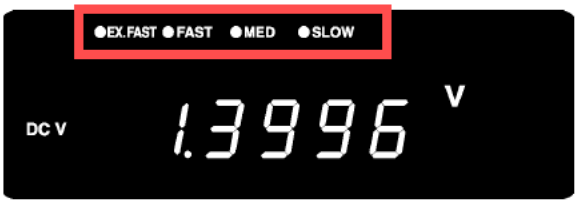

EX.FAST → FAST → MEDIUM → SLOW

NOTE

- Measurements are especially susceptible to interference from the environment when EX.FAST is selected, so countermeasures such as shielding or twisting of test leads, cables and wiring around the test object may be necessary.
- When SLOW sampling is selected, self-calibration is executed during each measurement. At other sampling rates, self-calibration is executed manually or automatically every 30 minutes.
  ❖See Section 4.9 Self-Calibration (Page 63).
- Refer to the specifications for details of sampling rates.
  ❖See Section Sampling Time (Page 158).

3.6 Zero-Adjust Function

Execute zero adjustment before measuring to nullify any residual offset voltage from the instrument or measurement environment. Measurement accuracy specifications are applicable after zero adjustment. Zero adjustment can also be executed by the 0ADJ terminal of the EXT I/O connector.
❖See Section 5.2 Signal Descriptions (Page 70).

3.6.1 Wiring Method for Zero-Adjustment

Before executing zero adjustment, connect the test leads (probes) as follows:

1. Connect SENSE-H to SENSE-L.
2. Connect SOURCE-H to SOURCE-L.
3. Connect the joined SENSE and SOURCE leads together as shown below.

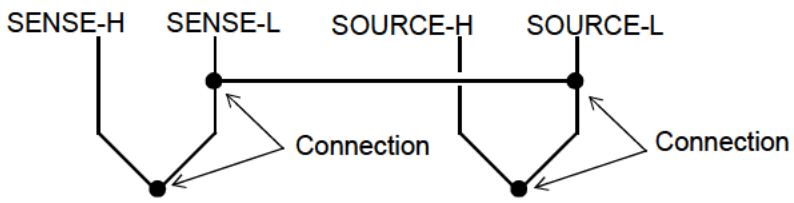

3.6.2 Executing Zero-Adjustment

1 **Short the test leads together.**
Proper zero adjustment is not possible with incorrect wiring.

Example: Model 9287-10 CLIP TYPE LEAD

Correct

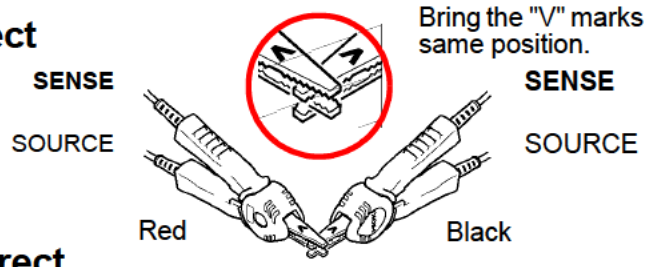

Incorrect

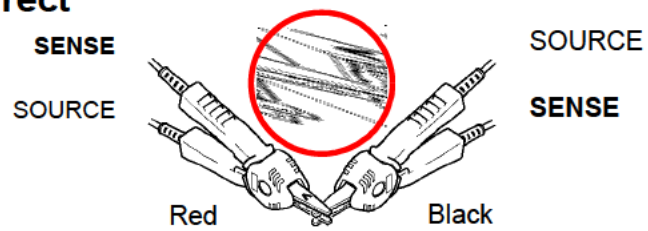

Model 9452 (Option)

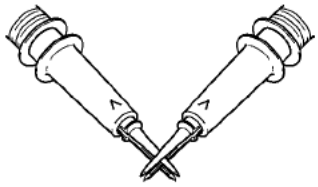

Model 9453 (Option)



Perform zero adjustment with the alligator clips and lead rods placed as above.

Model 9770 (Option)



2 SHIFT ○ **(SHIFT Lamp lit)**

↓

ΩV/Ω/V
0 ADJ

Zero-adjust display appears.

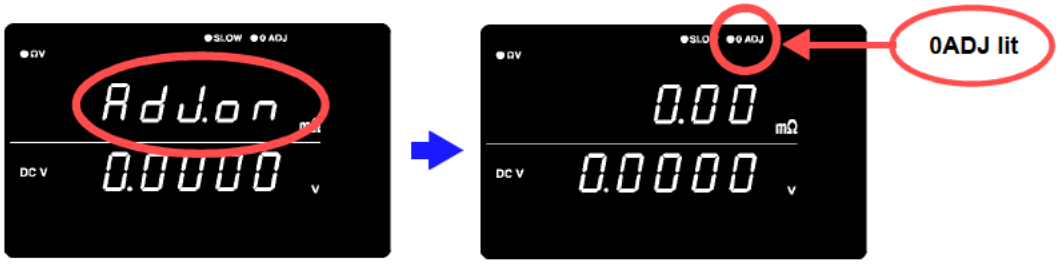

After measurement, the measured value of the compensation applied by the zero-adjust function is displayed.
The range of zero adjustment is up to 1,000 dgt.

Clearing Zero-Adjustment

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

(Main Display)

(Sub Display) flashing

2 ENTER

The zero-adjust value is cleared. (0ADJ not lit)

(Main Display)

If Err02 is displayed

Indicates that zero adjustment could not be executed, either because the range to be adjusted exceeds ± 1,000 dgt, or a measurement fault condition exists.
The zero adjust function is canceled, so repeat the operation after correcting the cause of the error.

NOTE

- Zero adjustment is limited to ± 1,000 dgt.
- Both resistance (all ranges) and voltage are adjusted together for all modes.
- Zero-adjustment values are retained even when power is turned off.
- The 0ADJ terminal of the EXT I/O connector also executes zero adjustment.
  ❖See Section 5.2 Signal Descriptions (Page 70).
- Zero adjustment is very difficult with the delicate probe tips of the Model 9455 and 9771 PIN TYPE LEADs. Refer to 3.6.1 Wiring Method for Zero-Adjustment (Page 28) to use other leads when executing zero adjustment.

3.7 Displaying Measurement Results

In the ΩV mode, resistance measurements appear on the upper display, and voltage measurements appear on the lower display.

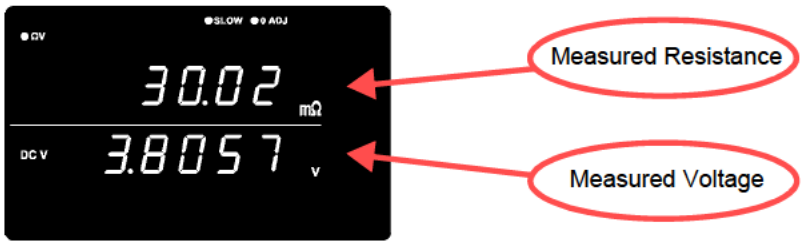

In the Ω mode, resistance measurements appear on the upper display.

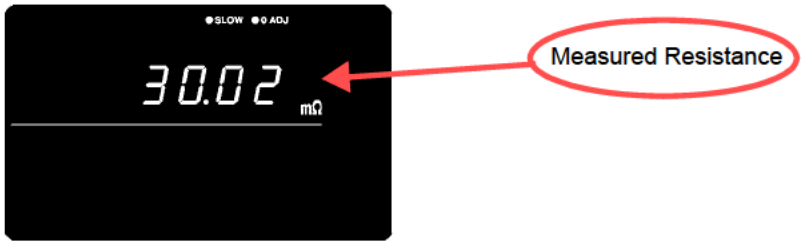

In the V mode, voltage measurements appear on the upper display.

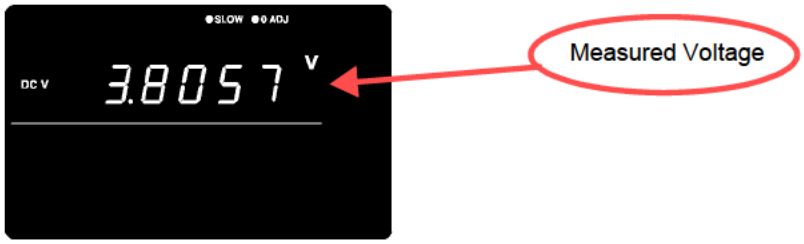

3.7.1 Measurement Fault Detection

If a measurement does not execute properly, a measurement fault "- - - - -" is indicated on the display.
In addition, a measurement fault signal (ERR) is output at the EXT I/O connector.
❖See Section 5.2.4 ERR Output (Page 73).

A measurement fault is displayed in the following cases.

- When a test lead is not connected to the test object
- When the resistance of the measured object is over-range
  Example: Attempting to measure 30 Ω with the 300 mΩ range selected.
- If any of the following is open, or has a bad connection: SOURCE-H, SOURCE-L, SENSE-H, SENSE-L
- When the resistance between SOURCE-H and SOURCE-L is 50 Ω or more in the 300 mΩ range (or 500 Ω or more in the 3 Ω range)
- When the resistance between SENSE-H and SENSE-L is greater than about 20 Ω. (However, if the capacitance of the test leads is 1 nF or higher, the measurement fault may not be detected.)
- When a bad contact results from damage, excessive wear or impurities on the test leads.
- If the circuit protection fuse is blown
  ❖See Section 9.1 Troubleshooting (Page 163).

3.7.2 Overflow Display

Overflow is indicated by "**OF**" or "**-OF**" on the display, caused by one of the following:

Display	Condition
OF	• The measured value exceeds the limit of the current measurement range • When the result of relative value calculation is larger than +99.999%.
-OF	• The measured value is below the limit of the current measurement range • When the result of relative value calculation is smaller than -99.999%.

Applied Measurement Chapter 4

This chapter describes advanced operations employing the Comparator, Statistical Calculation and Memory functions.

Judge measurement values against specified thresholds	Comparator Function	(34 page)
Measure when trigger events occur	Trigger Function	(51 page)
Output averaged measurement values	Averaging Function	(53 page)
Display the results of calculation expressions applied to measurement values	Statistical Calculation Functions	(54 page)
Store measurement values	Memory Function	(58 page)
Lock the keys	Key-Lock Function	(60 page)
Save measurement configurations	Panel Save Function	(61 page)
Load saved measurement configurations	Panel Load Function	(62 page)
Increase measurement precision	Self-Calibration	(63 page)
Output measurement values via the RS-232C interface according to trigger input timing	Measurement Value Output Function	(64 page)
Enable/disable key-press beeps	Key Beeper Setting	(65 page)
Re-initialize the instrument	Reset Function	(66 page)

4.1 Comparator Function

The comparator function compares measured values to preset upper and lower thresholds, judges the measurements according to their relative levels within the preset range, and indicates the results of the comparisons.
Comparator thresholds can be set either by specifying upper and lower thresholds, or by specifying a reference value and tolerance.
Comparator results can be indicated by the Hi, IN and Lo LEDs, beeper sound and signal output at the EXT I/O connector.
❖See Section Chapter 5 External Control (Page 69).

The comparator setting process flow is as follows:

1. Display the comparator settings
2. Set the comparator judgment beeper
3. Select the comparator execution mode (Auto or Manual/External)
4. Select resistance or voltage measurement
5. Select the comparison method (absolute or relative value) for the comparator
6. Specify the upper and lower thresholds (or reference value and tolerance)
7. Apply your comparator settings
8. Enable the Comparator function

4.1.1 Comparator Setting Example 1 (Upper and Lower Threshold Judgment)

This example describes the comparator setting method.

Example:
Set the upper and lower thresholds for resistance and voltage in the ΩV mode (300 mΩ range), and indicate whether the measurement value exceeds the upper or lower thresholds by sounding the beeper.

Resistance : Upper threshold value 150.00 mΩ, Lower threshold value 100.00 mΩ
Voltage : Upper threshold value 15.2000 V, Lower threshold value 15.0000 V

1 **Confirm that the Comparator function is OFF.**
First make sure the Comparator function is disabled. Settings cannot be changed while the Comparator function is enabled. Press the **COMP** key, if necessary, to disable the Comparator function.

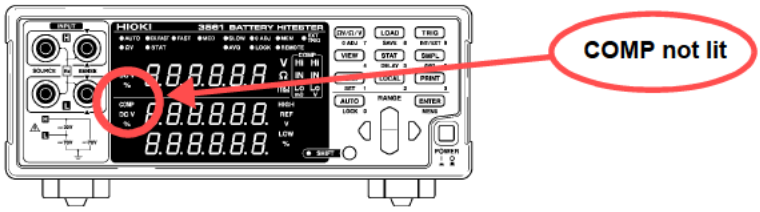

2 [ΩV/Ω/V] **Select the ΩV measurement mode.**

3 **Select the measurement range** (for this example, the 300 mΩ range).

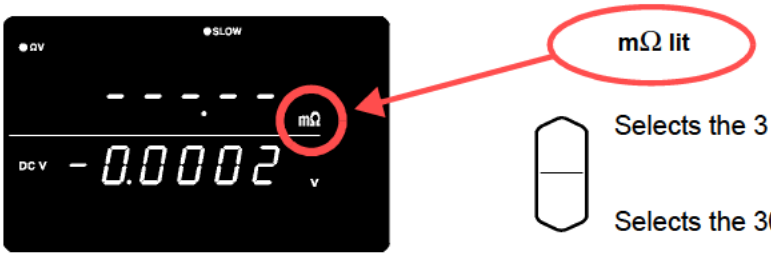

Selects the 3 Ω range (Ω lit)

Selects the 300 mΩ range (mΩ lit)

4 [SHIFT] → [COMP SET] **The Comparator setting display appears.**

5 **Set the comparator judgment beeper** (for this example, select HL).

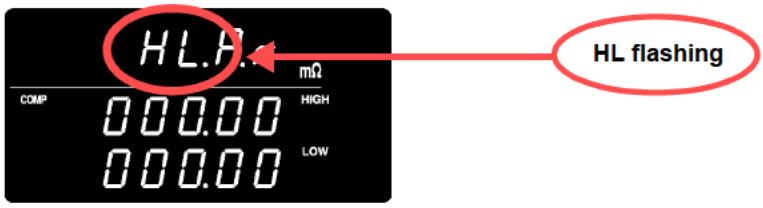

oFF.....no beeps sound
In .....beeps continuously (when measurements are IN)
HL.....beeps repeatedly (when measurements are Hi or Lo)
btH1.....beeps continuously while measurements are within the thresholds (IN), and beeps repeatedly when measurements are Hi or Lo.
btH2.....beeps once when measurements move into the threshold range (IN), and beeps repeatedly when measurements go Hi or Lo.

6 **Press so that the indicated position blinks, and select the comparator execution mode** (for this example, Auto).

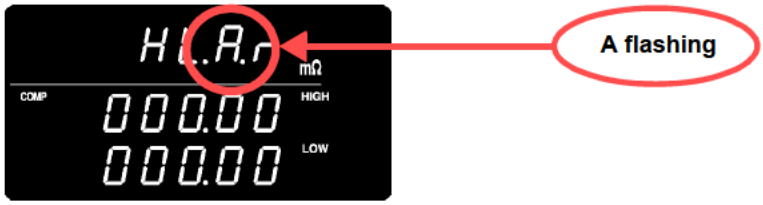

A..... Auto Comparator (default setting)
E..... Manual Comparator

7 **Press so that the indicated position blinks, and select resistance.**

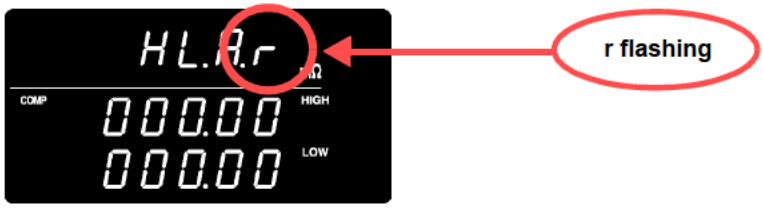

r.....Resistance
u.....Voltage

8 **Press so that the indicated position blinks, and select the comparison method for the comparator** (here, HIGH/LOW).

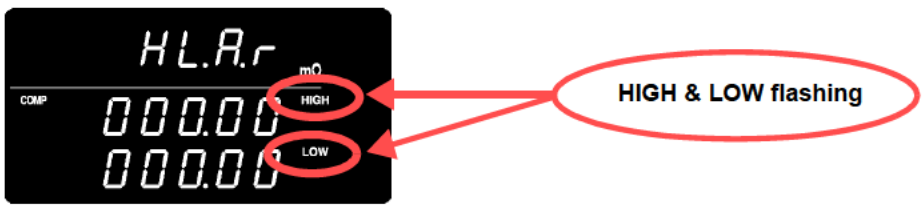

HIGH, LOW ..... Compare by upper and lower thresholds (default setting)
REF, %..... Compare by reference value and tolerance

9 **Switch to the upper/lower threshold setting display, and specify the thresholds.**

Or ten-keys

For this example,
Upper Threshold: 150 mΩ

Upper Threshold: 100 mΩ

Using the **RANGE** keys:	Using the ten-keys:
Select a digit to change by moving the blinking location, then select the new numerical value.	Press the numeric keys corresponding to the digits to be entered.
Select a digit	ΩV/Ω/V (0 ADJ 7) LOAD (SAVE 8) TRIG (INT/EXT 9) VIEW (4) STAT (DELAY 5) SMPL (AVG 6) COMP (SET 1) LOCAL (2) PRINT (3) AUTO (LOCK 0)
Select numerical value	

To enter the current measurement as the setting value: **AUTO** key
To enter the result of statistical calculation as the setting value: **STAT** key
❖See Section 4.1.6 Upper and Lower Thresholds Setting (by Reference Value and Tolerance) (Page 46).

10 **Press so that the indicated position blinks, and select voltage.**

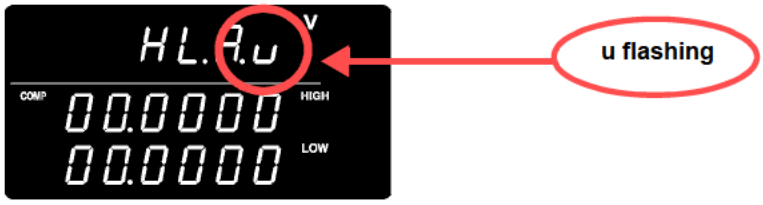

r ..... Resistance
u ..... Voltage

11 **Press so that the indicated position blinks, and select the comparison method for the comparator** (here, HIGH/LOW).

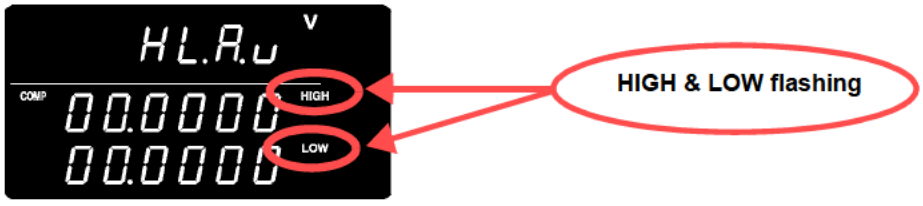

HIGH, LOW ..... Compare by upper and lower thresholds (default setting)
REF, % ..... Compare by reference value and tolerance

12

Switch to the upper/lower threshold setting display, and specify the thresholds.

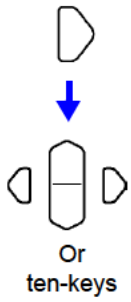

For this example,
Upper Threshold: 15.2 V

Upper Threshold: 15 V

13

ENTER

Applies setting and returns to the Measurement display.
The comparator function is enabled.

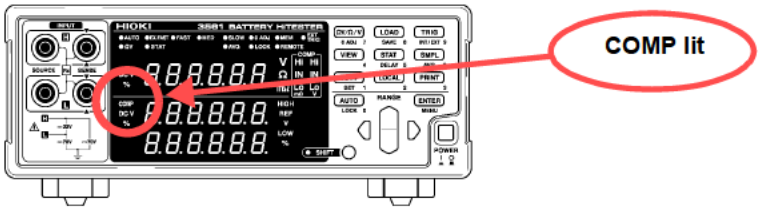

To cancel the settings: **SHIFT** key

14

Connect a test object and judge the measured value.

Measured Resistance

Judgment Result

Measured Voltage

In the ΩV mode, you can verify comparator settings by pressing the **VIEW** key.

❖See Section 4.1.9 Switching Between Measurement Value and Comparator Setting Displays (Page 50).



Upper Threshold Value < Measured Value

Lower Threshold Value ≤ Measured Value ≤ Upper Threshold Value

Measured Value < Lower Threshold Value

注記

The upper and lower thresholds are saved as the displayed counts (independent of measurement mode and range). Therefore, changing the measurement mode or range results in the same display counts representing different absolute values.
Example:
To specify the lower threshold as 150 mΩ in the 300 mΩ range, enter “15000”. Switching to the 3 Ω range after making this setting changes the lower threshold to 1.5 Ω.

4.1.2 Comparator Setting Example 2 (Reference Value and Tolerance Judgment)

This example describes the comparator setting method.

Example:
Set a reference value and tolerance in the ΩV mode (3 Ω range), and set the beeper to sound while measured values are within tolerance.

Resistance : Reference value 1.5 Ω, Tolerance 5%
Voltage : Reference value 4.2 V, Tolerance 0.5%

1 **Confirm that the Comparator function is OFF.**
First make sure the Comparator function is disabled. Settings cannot be changed while the Comparator function is enabled. Press the **COMP** key, if necessary, to disable the Comparator function.

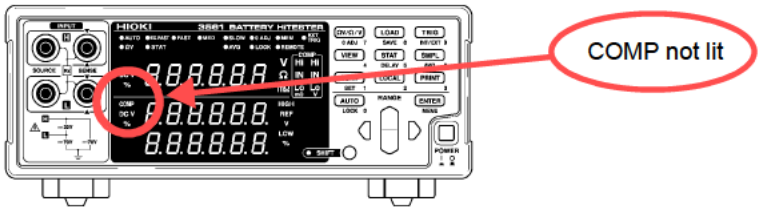

2 ΩV/Ω/V **Select the ΩV measurement mode.**

3 **Select the measurement range** (for this example, the 3 Ω range).

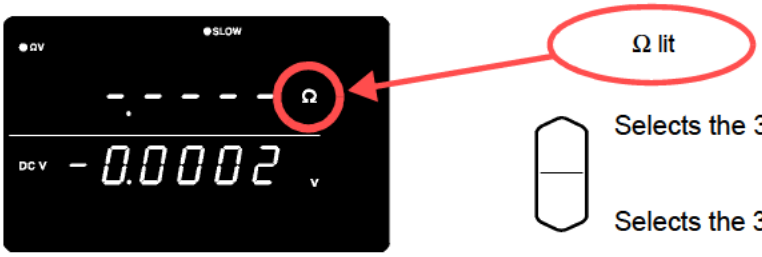

4 SHIFT → COMP SET **The Comparator setting display appears.**

5 **Set the comparator judgment beeper** (for this example, select In).

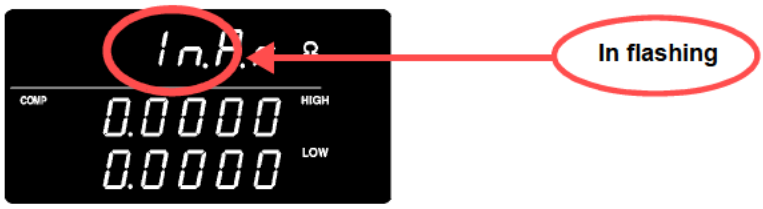

oFF.....no beeps sound
In .....beeps continuously (when measurements are IN)
HL.....beeps repeatedly (when measurements are Hi or Lo)
btH1.....beeps continuously while measurements are within the thresholds (IN), and beeps repeatedly when measurements are Hi or Lo.
btH2.....beeps once when measurements move into the threshold range (IN), and beeps repeatedly when measurements go Hi or Lo.

6 **Press so that the indicated position blinks, and select the comparator execution mode** (for this example, Auto).

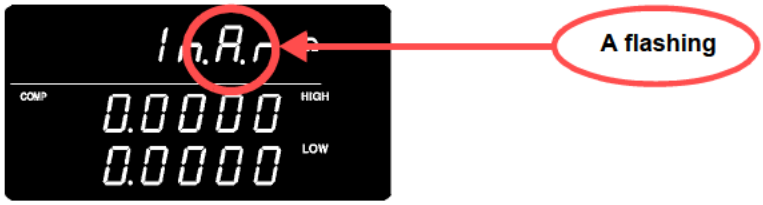

A..... Auto Comparator (default setting)
E..... Manual Comparator

7 **Press so that the indicated position blinks, and select resistance.**

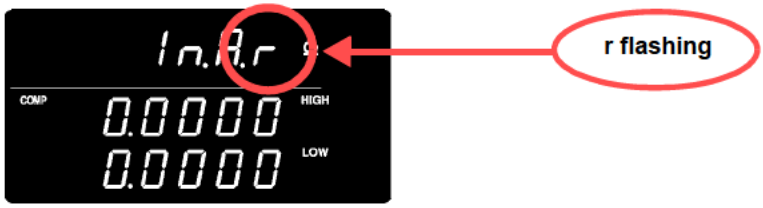

r.....Resistance
u.....Voltage

8 **Press so that the indicated position blinks, and select the comparison method for the comparator** (here, REF/%).

HIGH, LOW ..... Compare by upper and lower thresholds (default setting)
REF, %..... Compare by reference value and tolerance

9 **Switch to the Ref/% threshold setting display, and specify the thresholds.**



Relative (%) calculation expression

$$\frac{\text{Measured resistance - Reference value}}{\text{Reference value}} \times 100$$

For this example,
Reference value: 1.5 Ω

Tolerance: 5%

Using the **RANGE** keys:

Select a digit to change by moving the blinking location, then select the new numerical value.

Select a digit

Select numerical value

Using the ten-keys:

Press the numeric keys corresponding to the digits to be entered.



To enter the current measurement as the setting value: **AUTO** key
To enter the result of statistical calculation as the setting value: **STAT** key
❖See Section 4.1.6 Upper and Lower Thresholds Setting (by Reference Value and Tolerance) (Page 46).

10 **Press so that the indicated position blinks, and select voltage.**

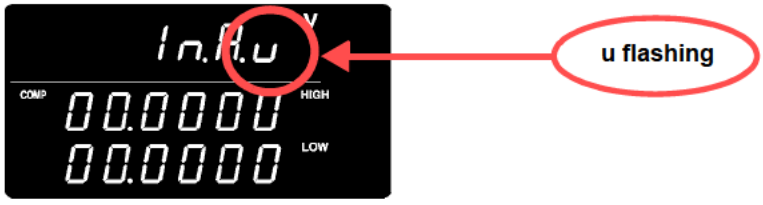

r..... Resistance
u..... Voltage

11 **Press so that the indicated position blinks, and select the comparison method for the comparator** (here, REF/%).

HIGH, LOW..... Compare by upper and lower thresholds (default setting)
REF, % ..... Compare by reference value and tolerance

12

Switch to the Ref/% threshold setting display, and specify the thresholds.

Or
ten-keys

Relative (%) calculation

$$\frac{\text{Measured voltage - Reference value}}{\text{Reference value}} \times 100$$

For this example,
Reference value: 4.2 V

Tolerance: 0.5%

13

ENTER

Applies setting and returns to the Measurement display.
The comparator function is enabled.

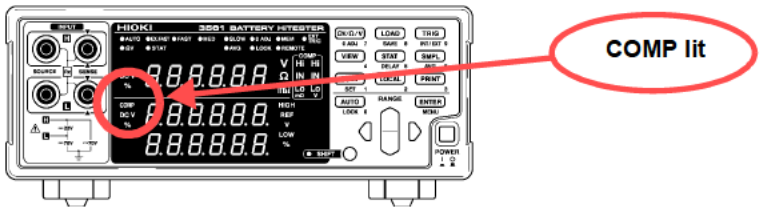

To cancel the settings: **SHIFT** key

14

Connect a test object and judge the measured value.

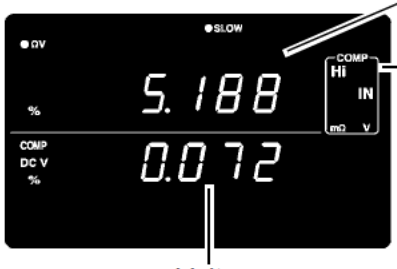

Resistance measurements are displayed as their relative percentage offset from the reference value (%)

Judgment Result

Relative percentage $= \frac{\text{Measured resistance - Reference value}}{\text{Reference value}} \times 100$

Voltage measurements are displayed as their relative percentage offset from the reference value (%)

In the ΩV mode, you can verify comparator settings by pressing the **VIEW** key.
❖See Section 4.1.9 Switching Between Measurement Value and Comparator Setting Displays (Page 50).

Upper Threshold Value of setting range < Measured value

Lower Threshold Value of setting range ≤ Measured value ≤ Upper Threshold Value of setting range

Measured value < Lower Threshold Value of setting range

4.1.3 Comparator Judgment Beeper Setting

Four beeper settings are available to audibly indicate comparator judgment results.

1 SHIFT **(SHIFT Lamp lit)**

↓

COMP SET **The Comparator setting display appears.**

2 **Set the comparator judgment beeper.**

(Main Display)

oFF.....no beeps sound
In .....beeps continuously (when measurements are IN)
HL.....beeps repeatedly (when measurements are Hi or Lo)
btH1 .....beeps continuously while measurements are within the thresholds (IN), and beeps repeatedly when measurements are Hi or Lo.
btH2 .....beeps once when measurements move into the threshold range (IN), and beeps repeatedly when measurements go Hi or Lo.

NOTE

- The beeper does not sound when the comparator judgment beeper setting is disabled (oFF).
- The beeper does not sound when there is no judgment result.
❖See Section 4.1.8 Comparator Judgment Results (Page 49).

4.1.4 Comparator Execution Mode Setting

Comparator judgment execution is selected by setting the auto or manual/external comparator mode. Comparator judgment can be enabled and disabled by EXT I/O signals. Refer to 5.2.2 Input Signals (Page 71).

1 SHIFT **(SHIFT Lamp lit)**

COMP SET **The Comparator setting display appears.**

2 **Press so that the indicated position blinks, and set the comparator execution mode.**

(Main Display)

A.....Auto comparator (comparator results are always output [default setting])

E.....Manual comparator (comparator results are output only when the MANU EXT I/O input is enabled [ON])

NOTE The auto setting is appropriate for normal use. Use the manual/external setting when you need to control comparator judgment timing.

4.1.5 Comparator Threshold Method Selection

Two methods are available for setting comparator thresholds.

1 SHIFT **(SHIFT Lamp lit)**

COMP SET **The Comparator setting display appears.**

2 **Press so that the indicated position blinks, and set the comparator threshold method.**

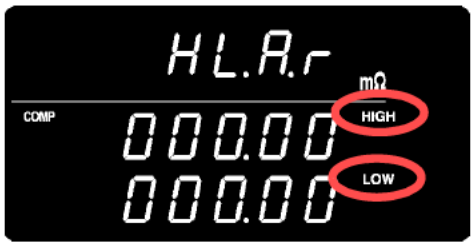

HIGH, LOW ..... Compare against specified upper and lower thresholds (default setting method)

REF, % ..... Compare against upper and lower thresholds internally calculated from a specified reference value and tolerance

About comparisons based on a reference value and tolerance

When the reference value and tolerance method is selected, thresholds are calculated as follows:

Upper threshold = reference value X (100 + tolerance [%]) / 100

Lower threshold = reference value X (100 - tolerance [%]) / 100

Measured values are displayed as a percentage relative to the reference value, calculated as follows:

Relative value = (measured value - reference value) / reference value X 100 [%]

4.1.6 Upper and Lower Thresholds Setting (by Reference Value and Tolerance)

1 SHIFT (SHIFT Lamp lit)

COMP SET

The Comparator setting display appears.

2 **Press so that the indicated position blinks, and select resistance or voltage.**

r .....Resistance
u .....Voltage

3 **Select the threshold setting display, and enter upper and lower threshold values.**

Or ten-keys

For example,
Upper Threshold: 150 mΩ
Lower Threshold: 100 mΩ

Using the **RANGE** keys:

Select a digit to change by moving the blinking location, then select the new numerical value.

Select a digit

Select numerical value

Using the ten-keys:

Press the numeric keys corresponding to the digits to be entered.



To enter the current measurement as the setting value: **AUTO** key

The current measurement value is set as the upper or lower threshold (during upper/lower threshold setting), or as the reference value (during reference value and tolerance setting). If the measured value is faulty or ± OF, it is ignored (not entered).

To enter a statistical calculation result as the setting value: **STAT** key

The result of statistical calculation is set as follows:

During upper/lower threshold setting	Upper threshold = average value + 3σ Lower threshold = average value - 3σ
During reference value and tolerance setting	Reference value = average value Tolerance = 3σ / average value X 100%

Where "σ" represents population standard deviation (σ_n).

No setting occurs if statistical calculation is disabled and no statistical calculation result exists.

❖See Section 4.4 Statistical Calculation Functions (Page 54).

Setting thresholds from the **AUTO** and **STAT** keys is possible only when the selected (blinking) character is non-numeric.

NOTE

Threshold and reference values can be set from 0 to 99999 (or 999999 for voltage), and tolerance can be set from 0.000 to 99.999%. Negative values are not settable. Entries using statistical calculation results that exceed the valid range are restricted to the range limit.

4.1.7 Enabling and Disabling the Comparator Function

COMP

Enables the comparator

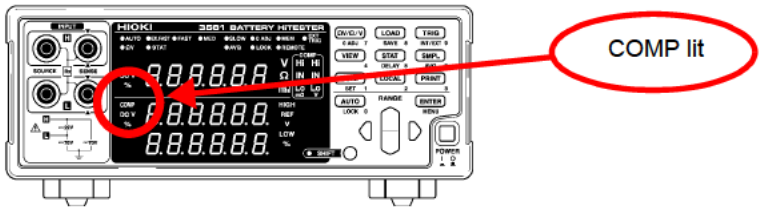

When the comparator is enabled, the following key operations are disabled to avoid inadvertent operations.

- **ΩV/Ω/V** key (Measurement mode setting)
- **SHIFT** → **ΩV/Ω/V** key (Zero-Adjustment)
- **SHIFT** → **COMP** key (Comparator setting)
- **AUTO** key (Auto-ranging setting)
- **SMPL** key (Sampling rate setting)
- **SHIFT** → **SMPL** key (Averaging setting)
- **SHIFT** → **TRIG** key (Trigger source setting)
- **SHIFT** → **ENTER** key (Menu display)
- **SHIFT** → **STAT** key (Delay setting)
- Range keys

NOTE

When the comparator is enabled, auto-ranging is automatically disabled.

4.1.8 Comparator Judgment Results

Resistance and voltage measurements are judged independently. Both judgment results are indicated on the display.

Judgment Operation

The comparator compares measured values with the preset threshold values, and judges whether the measurement is within the thresholds. Resistance and voltage measurements are judged independently.
The absolute value of the measurement is compared to the upper and lower thresholds.

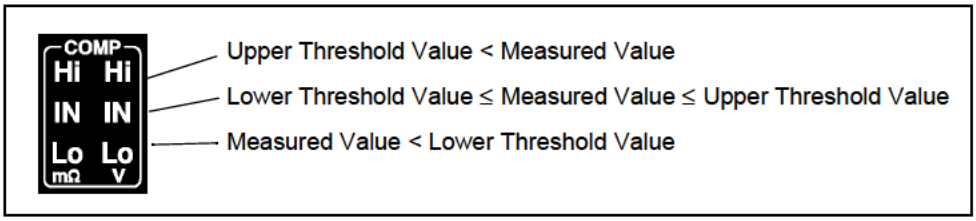

Measurement fault values are judged as follows:

Display	Judgment
- - - - -	No judgment
OF	Hi (exceeds the upper threshold)
-OF	Lo (less than the lower threshold)

AND Judgment Output

Judgment results (Hi, IN or Lo for both resistance and voltage) are output to EXT I/O connectors. Also, to facilitate application of judgment results, an AND output terminal indicates when both resistance and voltage are IN (within the threshold range).
❖See Section 5.2.3 Output Signals (Page 72).

NOTE

With the relative value comparison method (thresholds defined by a reference value and tolerance), the upper and lower thresholds are calculated internally for comparison with measurements. Therefore, even if a relative display value is equal to a judgment threshold (tolerance limit), it may be judged Hi or Lo.

4.1.9 Switching Between Measurement Value and Comparator Setting Displays

In ΩV mode, both resistance and voltage measurement values are displayed.
Although comparator setting values are not normally displayed when the comparator is enabled, they can be displayed for confirmation by the display switching function.

VIEW

Press this key to switch the display between measurement values and comparator setting values.

Resistance and voltage measurement display
(Shows resistance and voltage measurement values simultaneously)

Resistance measurement and comparator display
(Shows resistance measurement and resistance comparator setting values)

VIEW

Voltage measurement and comparator display
(Shows voltage measurement and voltage comparator setting values)

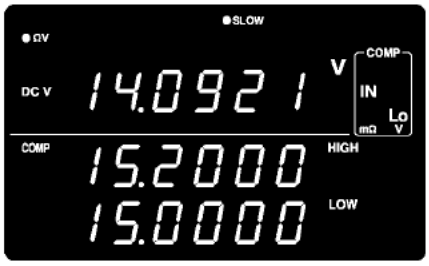

Measurement display switching is available only with the comparator enabled, and in the ΩV mode.

Use it to confirm comparator setting values.

4.2 Trigger Function

4.2.1 Trigger Source Settings

Two trigger sources are available: internal and external.

Internal Trigger	Trigger signals are automatically generated internally. (free-run)
External Trigger	Trigger signals are provided externally or manually.



(SHIFT Lamp lit)

Switches the selected trigger source.

EXT.TRIG lit.....External triggering is selected.
EXT.TRIG not lit.....Internal triggering is selected.

Measurement with External Triggering

An external trigger can be applied in three ways.

- Applying a trigger manually by operating key
  Pressing the TRIG key causes one measurement.
- Applying a trigger at the EXT I/O connector
  Grounding the $\overline{\text{TRIG}}$ terminal of the EXT I/O connector on the rear panel causes one measurement.
  ❖See Section 5.2.2 Input Signals (Page 71).
- Applying a trigger through RS-232C or GP-IB interface
  Sending the *TRG command via the RS-232C or GP-IB interface causes one measurement.

NOTE

- When Internal triggering is enabled, external input at the EXT I/O $\overline{\text{TRIG}}$ terminal and the *TRG command are ignored.
- The normal state of operation with the front panel controls is continuous measurement. Setting the trigger source to Internal enables the free-run condition in which triggering occurs continuously. When the trigger source is set to External, a measurement occurs each time an external trigger is applied. Continuous measurement can be disabled via RS-232C or GP-IB interface signals, in which case triggering occurs only when signaled by the external host (PC or PLC).
  ❖See Section Triggering System Description (Page 135).

4.2.2 Trigger Delay Settings

Specify the delay from the moment a trigger is applied to the start of measurement. By using this function, even when a trigger is applied immediately after connecting a test object, the start of measurement can be delayed to allow sufficient time for the measurement value to stabilize. Trigger delay can be set with 1 ms resolution from 0.000 to 9.999 seconds.

1 SHIFT → STAT (DELAY)

(SHIFT Lamp lit)

The Trigger Delay setting display appears.

(Main Display)

(Sub Display)
The current setting blinks.

2

Select ON.

(Sub Display)

3

The numerals indicating the trigger delay blink.

(Sub Display)

4 

Or ten-keys

Set the trigger delay.

5 ENTER

Applies setting and returns to the Measurement display.
To cancel the settings: SHIFT key

Disabling the Trigger Delay Function

1 SHIFT → STAT (DELAY)

(SHIFT Lamp lit)

The Trigger Delay setting display appears.

2

Select OFF.

(Sub Display)

3 ENTER

The Trigger Delay is disabled.

4.3 Averaging Function

The Averaging Function averages measurement values for output. This function can minimize instability of displayed values. The number of samples to average can be set from 2 to 16.

1 SHIFT → SMPL (AVG)

(SHIFT Lamp lit)

The Averaging Function setting display appears.

(Main Display)

(Sub Display)
The current setting blinks.

2

Select ON.

(Sub Display)

3

The number of samples to average setting blinks.

4

Or
ten-keys

Select the number of samples to average.

5 ENTER

The Average Measurement display appears. (AVG lit)
To cancel the settings: SHIFT key

Disabling the Averaging Function

1 SHIFT → SMPL (AVG)

(SHIFT Lamp lit)

The Averaging Function setting display appears.

2

Select OFF.

(Sub Display)

3 ENTER

The Averaging Function is disabled. (AVG not lit)

NOTE

When the internal trigger is used for continuous measurement (free-run), the display shows the moving average. Otherwise, the display shows the integrating average.
❖See Section 4.2 Trigger Function (Page 51).

4.4 Statistical Calculation Functions

The mean, maximum, minimum, standard deviation of population, standard deviation of sample and process capability indices are calculated and displayed for up to 30,000 measurement values.

The calculation formulas are as follows:

Mean

$$\bar{x} = \frac{\sum x}{n}$$

Standard deviation of population

$$\sigma = \sqrt{\frac{\sum x^2 - n\bar{x}^2}{n}} \quad (= \sigma_n)$$

Standard deviation of sample

$$s = \sqrt{\frac{\sum x^2 - n\bar{x}^2}{n-1}} \quad (= \sigma_{n-1})$$

Process capability index (dispersion)

$$Cp = \frac{|Hi - Lo|}{6\sigma_{n-1}}$$

Process capability index (bias)

$$CpK = \frac{|Hi - Lo| - |Hi + Lo - 2\bar{x}|}{6\sigma_{n-1}}$$

- In these formulas, n represents the number of valid data samples.
- Hi and Lo are the upper and lower thresholds of the comparator.
- The process capability indices represent the quality achievement capability created by a process, which is the breadth of the dispersion and bias of the process' quality. Generally, depending on the values of Cp and CpK, process capability is evaluated as follows:
  Cp, CpK>1.33..... Process capability is ideal
  1.33 ≥ Cp, CpK>1.00..... Process capability is adequate
  1.00 ≥ Cp, CpK..... Process capability is inadequate

NOTE

- When only one valid data sample exists, standard deviation of sample and process capability indices are not displayed.
- When σ_{n-1} is 0, Cp and CpK are 99.99.
- The upper limit of Cp and CpK is 99.99. Values of Cp and CpK>99.99 are displayed as 99.99.
- Negative values of CpK are handled as CpK=0.
- When comparator, range or auto-ranging settings are changed while statistical data is displayed, the display of Cp and CpK values changes to "- - . - -".
- When normal measurement values and relative display values (%) are mixed, correct calculation results cannot be obtained.

Enabling/Disabling the Statistical Calculation Function

1 STAT **The Statistical Calculation display appears.**

(Main Display)

(Sub Display)

2 (press three times) **The function enable/disable display appears.**

(Sub Display)

Enable or disable the Calculation Function on the Sub Display.
on..... enables the calculation function (ON).
off ..... disables the calculation function (OFF).

3 ENTER **Applies setting and returns to the Measurement display.**
To cancel the settings: SHIFT key

NOTE

- Statistical Calculation function setting (ON, OFF) is not available when the Comparator is enabled.
- If Statistical Calculation is turned off and then back on without first clearing calculation results, it resumes calculating from the point when it was turned off.
- The Statistical Calculation function slows measurements when it is ON.

Clearing Statistical Calculation Results

1 STAT **The Statistical Calculation display appears.**

(Main Display)

(Sub Display)

2 (press once) **The Clearing screen will appear.**

(Sub Display)

3 ENTER **Clears statistical calculation results.**

Automatic Clearing of Statistical Calculation Results after Printing

The instrument can be set to automatically clear statistical calculation results after results are output to the printer.

1 STAT **The Statistical Calculation display appears.**

(Main Display)

(Sub Display)

2 (Press twice) **Bring up Auto Clearing After Printing in the Setup screen.**

(Sub Display)

3 **Turn Automatic Clearing After Printing on or off.**
on..... Automatically clears statistical calculation results after they are output to the printer.
off..... Does not clear the results themselves.

4 ENTER **Applies setting and returns to the Measurement display.**
To cancel the settings: SHIFT key

Importing Data

TRIG Pressing the **TRIG** key while Statistical Calculation is ON executes one of the following operations:

- External Trigger: Takes one measurement and performs statistical calculation on the result
- Internal Trigger: Performs statistical calculation on the value displayed immediately after pressing

NOTE
- *TRG command executes the same operation.
- Grounding the $\overline{\text{TRIG}}$ terminal of the EXT I/O connector executes the same operation.

Confirming Statistical Calculation Results

1 STAT **The Statistical Calculation display appears.**

2 The indication on the display changes as follows with each key-press.

Example: when the ΩV mode is selected
(not displayed in V mode)

Total data count of resistance measurement

Mean of resistance measurement

Valid data Mean

Maximum of resistance measurement

Maximum Data Sample No.

Minimum of resistance measurement

Minumum Data Sample No.

Standard deviation of population of resistance measurement

Standard deviation of sample of resistance measurement

Process capability indices of resistance measurement

Cp
CpK

(not displayed in Ω mode)

Total data count of voltage measurement → Mean of voltage measurement → Maximum of voltage measurement

Minimum of voltage measurement → Standard deviation of population of voltage measurement → Standard deviation of sample of voltage measurement

Process capability indices of voltage measurement

ON/OFF setting

Auto Clearing After Printing setup

Clear setup

NOTE

- When a valid data count (measurement fault other than ± OF) is zero, no calculation result is displayed.
- When only one valid data sample exists, standard deviation of sample and process capability indices cannot be displayed.
- When comparator, range or auto-ranging settings are changed while statistical data is displayed, the display of Cp and CpK values changes to "- - . - -".

Sending Statistical Calculation Results to the Printer

PRINT

With the statistical calculation results displayed, press the PRINT key. The statistical calculation results are output to the optional printer.

❖See Section Chapter 6 Printer (Optional) (Page 79).

4.5 Memory Function

The Memory function is only available via communication commands. When the Memory function is enabled, measurement values are stored in the instrument's internal memory according to trigger input sequence (up to 400 values). Stored data can be downloaded later upon command.
When measuring using a scanner to switch multiple test objects, switching time can be quite long if measurement values are downloaded to the PC after each measurement. Test cycle time can be minimized by using this function to store measurement values internally until all channel measurements are finished, at which time the stored values are downloaded together during the next idle period.

1 **Select the RS-232C or GP-IB interface.**
❖See Section 7.3.2 Selecting the Interface (Page 91).

2 **Send the command to enable the Memory function.**
`:MEMory:STATe ON`

3 **The MEM indicator lights.**

4 **Measurement values are stored.**
When a trigger is applied by the **TRIG** key, $\overline{\text{TRIG}}$ EXT I/O input signal or `*TRG` command, the MEM indicator blinks once and the measured value is stored.

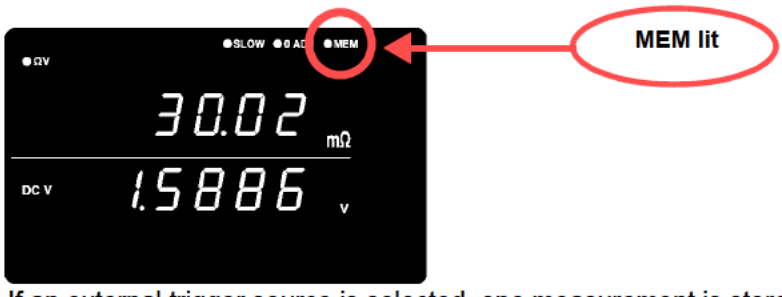

If an external trigger source is selected, one measurement is stored after each trigger event. In the internal triggering case, the first measurement value after triggering is stored. Apply a trigger as many times as is necessary.

5 **Send the command to download the data from memory.**

```
:MEMory:DATA?
```

The stored measurement values are returned in response.

```
:MEM:DATA?
1,   290.60E-3,   1.3924E+0
2,   290.54E-3,   1.3924E+0
3,   290.50E-3,   1.3923E+0
4,   290.43E-3,   1.3923E+0
5,   290.34E-3,   1.3924E+0
END
```

The "END" character is sent as the last line of the data.

To download stored data one measurement at a time, send this command:

```
:MEMory:DATA? STEP
```

The instrument sends one stored data object and enters the wait state.
When the instrument receives an "N" from the PC or other device, the next stored data object is sent.
Repeat until the last data object is downloaded.
When all stored data has been downloaded, the instrument sends an "END" character.

```
:MEM:DATA? STEP
1,   290.60E-3,   1.3924E+0
N                          (sent from PC)
2,   290.54E-3,   1.3924E+0
N                          (sent from PC)
3,   290.50E-3,   1.3923E+0
N                          (sent from PC)
4,   290.43E-3,   1.3923E+0
N                          (sent from PC)
5,   290.34E-3,   1.3924E+0
N                          (sent from PC)
END
```

6 **To clear the instrument's memory, send it the following command.**

```
:MEMory:CLEAr
```

Unless the memory is cleared, measurement data continues to be stored upon each trigger event.

NOTE

- The instrument's memory storage capacity is 400 measurements. Be aware that attempting to store more data (by applying a trigger) results in nothing further being stored.
- Refer to Chapter 7 RS-232C/GP-IB Interfaces (Page 87), for details about the communication methods and sending and receiving commands.
- When the Memory function is enabled, auto-ranging is not available.
- Memory contents are cleared when performing the following operations:
  When enabling the Memory function (off to on)
  When changing the measurement range
  When changing comparator settings
  When sending the `:Memory:Clear` command
  When Reset is executed from the menu display
  When sending `*RST`
  When sending `:SYSTem:RESet`
  When turning power on

4.6 Key-Lock Function

Executing Key-Lock disables the operating keys on the front of the instrument. This function can be useful for protecting settings.



(SHIFT Lamp lit)

Enable the Key-Lock function.

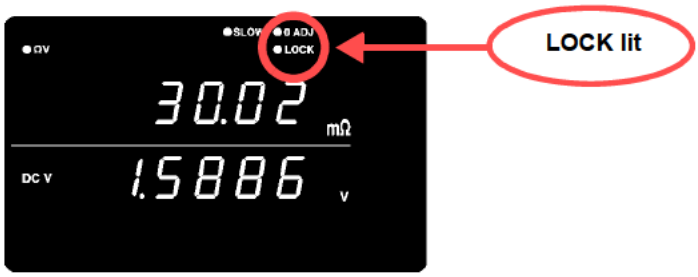

NOTE

- Even if the power supply is interrupted, the Key-Lock function is not canceled.
- The **TRIG** key remains operational.

Disabling Key-Lock



(SHIFT Lamp lit)

Disable the Key-Lock function. (LOCK is not lit)

NOTE

When communicating by remote control, the remote control status is canceled.

4.7 Panel Save Function

The current measurement setting state is stored (saved) in non-volatile memory.
Up to 126 sets of measurement states can be saved.
The measurement settings (state) at the time this function is executed are saved.
Saved measurement states can be reloaded using the Panel Load function, described later.

1 SHIFT → LOAD / SAVE

(SHIFT Lamp lit)

The Panel Saving display appears.

(Main Display)

(Sub Display)
The panel number blinks.

2 Or ten-keys

Select the panel number to save.

(Sub Display)
(To save measurement settings as Panel No. 3)

When selecting a saved panel, "**USEd**" is displayed.

3 ENTER

Saves the measurement setting state and returns to the Measurement display.
To cancel the settings: SHIFT key

NOTE

- If you select a Panel number that was previously saved and press the **ENTER** key, the contents are overwritten.
- The Key-Lock state can be saved only by the `:SYSTem:SAVE` remote command.

Saved Items

- Measurement mode setting
- Range setting
- Auto-ranging setting
- Sampling rate setting
- Comparator settings
- Internal/External trigger setting
- Switching displays setting
- Delay setting
- Zero-Adjust setting
- Averaging setting
- Key-Lock
- Statistical Calculation setting

4.8 Panel Load Function

Loads the measurement settings saved by the Panel Save function from internal non-volatile memory.

1 LOAD

The Panel Loading display appears.

(Main Display)

(Sub Display)
The panel number blinks.

2 Or ten-keys

Select the panel number to load.

(Sub Display)
(To load measurement settings from Panel No.3)

3 ENTER

Loads the measurement setting state and returns to the Measurement display.
To cancel the settings: SHIFT key

NOTE

- If an unsaved Panel No. is selected, a warning beep sounds when you press **ENTER** key.
- When selecting a Panel No. with the up/down **RANGE** keys, only the numbers of previously saved panels appear.
- Loading can also be executed using the $\overline{\text{TRIG}}$ signal and the $\overline{\text{LOAD0}}$ to $\overline{\text{LOAD6}}$ pins of the EXT I/O interface.
  ❖See Section 5.2.2 Input Signals (Page 71).

4.9 Self-Calibration

The self-calibration function adjusts offset voltage and gain drift of the instrument's internal circuitry to improve measurement precision.
The instrument's measurement accuracy specifications depend on self-calibration, so it must be executed frequently. In particular, always execute self-calibration after warm-up and when the ambient temperature changes by more than 2°C. However, regardless of this setting, self-calibration is executed during every measurement when SLOW sampling is used.

Self-calibration can be executed by the following two methods:

Auto	Executes self-calibration automatically once every 30 minutes.
Manual	Self-calibration can be executed manually by applying a $\overline{\text{CAL}}$ input signal (grounding the $\overline{\text{CAL}}$ terminal of the EXT I/O connector).

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

The Self-Calibration setting display appears.
❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).

(Main Display)

(Sub Display)
The current setting blinks.

3

Select Auto or Manual on the Sub Display.
AUto ..... Auto self-calibration
In..... Manual self-calibration

4 ENTER

Applies setting and returns to the Measurement display.

NOTE

Self-calibration requires about 55 ms, during which measurement processing is temporarily suspended.

4.10 Measurement Value Output Function

This function causes output of measured values via the RS-232C interface in the same sequence as trigger input.
This function is useful when measuring using internal (free-run) triggering, and for obtaining measured values on a PC when using a footswitch for triggering.

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

The Measurement Value Output function setting display appears.
❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).

(Main Display)

(Sub Display)
The current setting blinks.

3

Turn Measurement Value Output Function on or off.
on..... enables the measurement value output function (ON).
off..... disables the measurement value output function (ON).

4 ENTER

Applies setting and returns to the Measurement display.

5 TRIG

The measured value is output from the RS-232C interface when you press the TRIG key or when a signal is applied to the EXT I/O TRIG terminal.
Set the PC to the receiving state beforehand. When a measurement value is received, the PC should perform appropriate processing such as recording or displaying, then re-enable the receiving state.

NOTE

- When external triggering is enabled, a measurement is performed and the value is sent after each trigger event. When internal triggering is enabled, the first value measured after triggering is sent.
- The measurement output function is not applicable to the GP-IB interface or printer.

4.11 Key Beeper Setting

Select whether a beep sounds when an operating key on the front of the instrument is pressed.

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

The Key Beeper setting display appears.
❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).

(Main Display)

(Sub Display)
The current setting blinks.

3

Select the key beeper state on the Sub Display.
on..... Key beeper enabled
off ..... Key beeper disabled

4 ENTER

Applies setting and returns to the Measurement display.

4.12 Reset Function

The reset function can be used to re-initialize current measurement settings (excluding saved panel data) to their factory defaults, or to re-initialize all measurement settings including saved panel data to factory defaults.

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

The Reset display appears.

❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).



(Main Display)

(Sub Display)
The current setting blinks.

3

Select the Reset method on the Sub Display.

SEt ..... Reset (initializes measurement settings other than those stored with Panel Save)

SYS ..... System Reset (initialize all measurement settings)

4

ENTER blinks.

(Sub Display)

When SYS (system reset) is selected

5 ENTER

Executes the Reset.

To cancel the settings: SHIFT key

NOTE System Reset also initializes Panel Save data.

Initial Factory Default Settings

Description	Default
Measurement Mode	ΩV
Resistance Measurement Range	AUTO
Zero-Adjust	OFF
Zero-Adjust Value	0
Delay	OFF
Delay Time	0.000s
Sampling Rate	SLOW
Averaging Function	OFF
Average Times	2
Self-Calibration	AUTO
Continuous Measurement	ON
Trigger Source	Internal trigger
Line Frequency	50 Hz
Key Beeper Setting	ON
Key-Lock Function	OFF
Comparator	OFF
Comparator Threshold Method (resistance and voltage)	Hi, Lo
Comparator Upper Threshold (resistance and voltage)	0
Comparator Lower Threshold (resistance and voltage)	0
Comparator Judgment Beeper	OFF
Comparator Execution Mode	AUTO
Statistical Calculation Functions	OFF
Automatic Clearing of Statistical Calculation Results	OFF
Interface	RS-232C
Baud Rate	9600 bps
GP-IB Address	1
GP-IB Delimiter	LF
Print Interval	0 (The interval print disabled)
Error Output	ASync
Measurement Value Output Function	OFF
EOC Output	HOLD
EOC Pulse Width	1 ms

External Control Chapter 5

5.1 Overview

External Control Input Functions

- External trigger input (TRIG)
- Select Panel No. to load (LOAD0 to LOAD6)
- Zero-adjust signal input (0ADJ)
- Print Signal input (PRINT)
- Self-calibration signal input (CAL)
- Manual comparator judgment input (MANU)

External Output Terminal Functions

- End-of-Conversion signal output (EOC)
- Reference signal output (INDEX)
- Measurement Fault signal output (ERR)
- Comparator decision signal output (R-Hi, R-IN, R-Lo, V-Hi, V-IN, V-Lo, AND)
- General-purpose outputs (OUT0 to OUT9)

Connector Type

57RE-40360-730B (D29) (manufactured by DDK)

Mating Connector

57-30360 (manufactured by DDK)
RC30-36P (manufactured by HIROSE electric co.,ltd.)
or equivalent

⚠WARNING

To avoid electric shock or damage to the equipment, always observe the following precautions when connecting to EXT I/O connector.

- **Always turn off the power to the instrument and to any devices to be connected before making connections.**
- **Be careful to avoid exceeding the ratings of EXT I/O connector.**
- **During operation, a wire becoming dislocated and contacting another conductive object can be serious hazard. Make sure that connections are secure the EXT I/O connectors.**
- **The INT.GND terminals (Page 71) are grounded, so if an external controller has a potential relative to ground, connection could cause a short-circuit accident.**

⚠CAUTION

Be aware of the following to avoid damaging the instrument:

- When using relays, always include diodes to absorb back emf.
- Always provide protective grounding for devices the connect to the EXT I/O connectors.

5.2 Signal Descriptions

5.2.1 Pinout

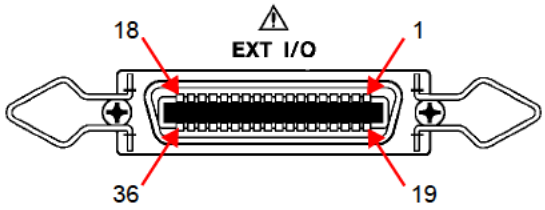

EXT I/O Connector

Pin	I/O	Signal name	Pin	I/O	Signal name
1	IN	$\overline{\text{LOAD0}}$	19	IN	$\overline{\text{LOAD1}}$
2	IN	$\overline{\text{LOAD2}}$	20	IN	$\overline{\text{LOAD3}}$
3	IN	$\overline{\text{LOAD4}}$	21	IN	$\overline{\text{LOAD5}}$
4	IN	$\overline{\text{LOAD6}}$	22	IN	$\overline{\text{TRIG}}$ ($\overline{\text{IN0}}$)
5	IN	$\overline{\text{CAL}}$ ($\overline{\text{IN1}}$)	23	IN	$\overline{\text{0ADJ}}$ ($\overline{\text{IN2}}$)
6	IN	$\overline{\text{PRINT}}$ ($\overline{\text{IN3}}$)	24	IN	$\overline{\text{MANU}}$ ($\overline{\text{IN4}}$)
7	–	INT.GND	25	–	INT.GND
8	–	INT.GND	26	–	INT.GND
9	OUT	R-Hi	27	OUT	R-IN
10	OUT	R-Lo	28	OUT	AND
11	OUT	V-Hi	29	OUT	V-IN
12	OUT	V-Lo	30	OUT	ERR
13	OUT	EOC	31	OUT	INDEX
14	OUT	OUT0	32	OUT	OUT1
15	OUT	OUT2	33	OUT	OUT3
16	OUT	OUT4	34	OUT	OUT5
17	OUT	OUT6	35	OUT	OUT7
18	OUT	OUT8	36	OUT	OUT9

5.2.2 Input Signals

$\overline{\text{LOAD0}}$ to $\overline{\text{LOAD6}}$

Select a Panel No. to load and apply a $\overline{\text{TRIG}}$ signal to load the selected Panel No. and measure. $\overline{\text{LOAD0}}$ is the LSB, and $\overline{\text{LOAD6}}$ is the MSB.
When a TRIG signal is applied, if $\overline{\text{LOAD0}}$ through $\overline{\text{LOAD6}}$ are unchanged from the previous trigger event, panel settings are not loaded. In this case, using external triggering, one measurement is taken as usual when the $\overline{\text{TRIG}}$ signal is applied.

Panel No.	$\overline{\text{LOAD6}}$	$\overline{\text{LOAD5}}$	$\overline{\text{LOAD4}}$	$\overline{\text{LOAD3}}$	$\overline{\text{LOAD2}}$	$\overline{\text{LOAD1}}$	$\overline{\text{LOAD0}}$
*	1	1	1	1	1	1	1
1	1	1	1	1	1	1	0
2	1	1	1	1	1	0	1
3	1	1	1	1	1	0	0
4	1	1	1	1	0	1	1
5	1	1	1	1	0	1	0
6	1	1	1	1	0	0	1
7	1	1	1	1	0	0	0
8	1	1	1	0	1	1	1
...							
122	0	0	0	0	1	0	1
123	0	0	0	0	1	0	0
124	0	0	0	0	0	1	1
125	0	0	0	0	0	1	0
126	0	0	0	0	0	0	1
*	0	0	0	0	0	0	0

0: $\overline{\text{LOAD}}$ terminal is shorted to GND 1: $\overline{\text{LOAD}}$ terminal is unconnected, or connected to 5 V

* When a $\overline{\text{TRIG}}$ signal is applied with $\overline{\text{LOAD0}}$ to $\overline{\text{LOAD6}}$ set to all 1's or all 0's, no Panel Load occurs.

At least 70 ms is required for the settings to change after executing a Panel Load.

$\overline{\text{TRIG}}$

When the external trigger, one measurement is taken each time the $\overline{\text{TRIG}}$ signal transitions from High to Low.
This trigger signal is ignored when internal triggering is enabled.
Trigger functions are also available for statistical calculation, recording to memory and output of measured values (valid also with internal triggering).

$\overline{\text{CAL}}$

When manual self-calibration is selected with EX.FAST, FAST or MEDIUM sampling rate, self-calibration begins when the $\overline{\text{CAL}}$ signal transitions from High to Low.
Self-calibration takes about 55 ms.
When SLOW sampling is selected, the $\overline{\text{CAL}}$ signal is ignored.
❖See Section 4.9 Self-Calibration (Page 63).

$\overline{\text{0ADJ}}$ — Zero adjustment executes once when the $\overline{\text{0ADJ}}$ signal transitions from High to Low.

$\overline{\text{PRINT}}$ — The current measurement value prints when the $\overline{\text{PRINT}}$ signal transitions from High to Low.

$\overline{\text{MANU}}$ — When the MANU comparator mode is selected, comparator judgment is enabled while the $\overline{\text{MANU}}$ signal is Low.
❖See Section 4.1.4 Comparator Execution Mode Setting (Page 44).

$\overline{\text{IN0}}$ to $\overline{\text{IN4}}$ — The $\overline{\text{TRIG}}$, $\overline{\text{CAL}}$, $\overline{\text{0ADJ}}$, $\overline{\text{PRINT}}$ and $\overline{\text{MANU}}$ signals can also serve as general-purpose input terminals, read with the **`:IO:IN?`** command.
❖See Section EXT I/O Input (Page 134).

5.2.3 Output Signals

ERR — Indicates a measurement fault.
The Synchronous ERR output setting causes ERR output to be synchronous with EOC output, while with the Asynchronous ERR output setting causes ERR output to follow actual (asynchronous) contact of the probes with the test object.
❖See Section 5.2.4 ERR Output (Page 73).

INDEX — The INDEX signal is output during the Trigger Wait, Delay, Self-Calibration and Calculation states.
This signal is not output while measuring the resistance of test objects.
This signal transitions from Off to On to indicate that the test object can be removed.

EOC — This signal indicates the end of a measurement (End-Of-Conversion).
This signal indicates when comparator judgment results and ERR output (when SYNC is enabled) are available.

R-Hi, R-IN, R-Lo
V-Hi, V-IN, V-Lo — These are the results of comparator decision.

AND — This signal indicates when both resistance and voltage judgment results are IN (ΩV mode).
In the Ω and V modes, this signal is the same as R-IN and V-IN outputs, respectively.

OUT0 to OUT9 — The output signals are controlled by the **`:IO:OUT`** command.
❖See Section EXT I/O Output (Page 134).

INT.GND — This is the instrument's internal ground.

NOTE

- I/O signals should not be used while measurement settings have been changed.
- The EOC and INDEX signals are initialized (ON) at power on.
- If it is not necessary to change the measurement conditions, set $\overline{\text{LOAD0}}$ through $\overline{\text{LOAD6}}$ to either Hi or Lo.

5.2.4 ERR Output

The ERR output signal indicates the occurrence of measurement fault conditions (such as open test leads, or a bad contact).
There are two ERR output methods.

Synchronized with EOC Output (SYNC)

Measurement faults detected while measuring (not while awaiting trigger or during delay or calculation intervals), are indicated by ERR output synchronous with EOC output (the end-of-measurement signal).

ERR Output On: A measurement fault has prevented correct measurement
ERR Output Off: Correct measurement obtained (OF or -OF: Out-of-range cases are included)

Asynchronous with EOC Output (ASYNC)

Measurement faults (test lead connection conditions) are output in real time. The output is asynchronous with the $\overline{\text{TRIG}}$ signal and EOC output.

ERR Output On: Measurement fault condition (open test leads, or a bad contact)
ERR Output Off: Test lead connections are normal

5.2.5 Instrument Settings

Measurement Fault Output Signal (ERR) Setting

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2 ▷

Select the ERR Output Selection display.

❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).



(Main Display)

(Sub Display)
The current setting blinks.

3 ▷

Select the type of signal to be output on the Sub Display.

SynC ..... Synchronous output (synchronized with EOC output)
ASynC ..... Asynchronous output (not synchronized with EOC output)

4 ENTER

Applies settings and returns to the Measurement display.

Setting the EOC Signal

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2 ▷

Select the EOC-signal setup display.

❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).



(Main Display)

(Sub Display)
The current setting blinks.

3 ▷

Choose the output method for the EOC signal.

HoLd ..... Holds the EOC signal after measurement.
→ Go to Step 5.
PULSE ..... Outputs the specified pulse after measurement.
→ Go to the next step.

4 ◁ ▷ Or ten-keys

(When PULSE is selected)
The number representing the pulse width of the EOC signal will start blinking.
Set the pulse width in ms.

5 ENTER

Applies settings and returns to the Measurement display.

5.3 Timing Chart

External Trigger Timing Chart

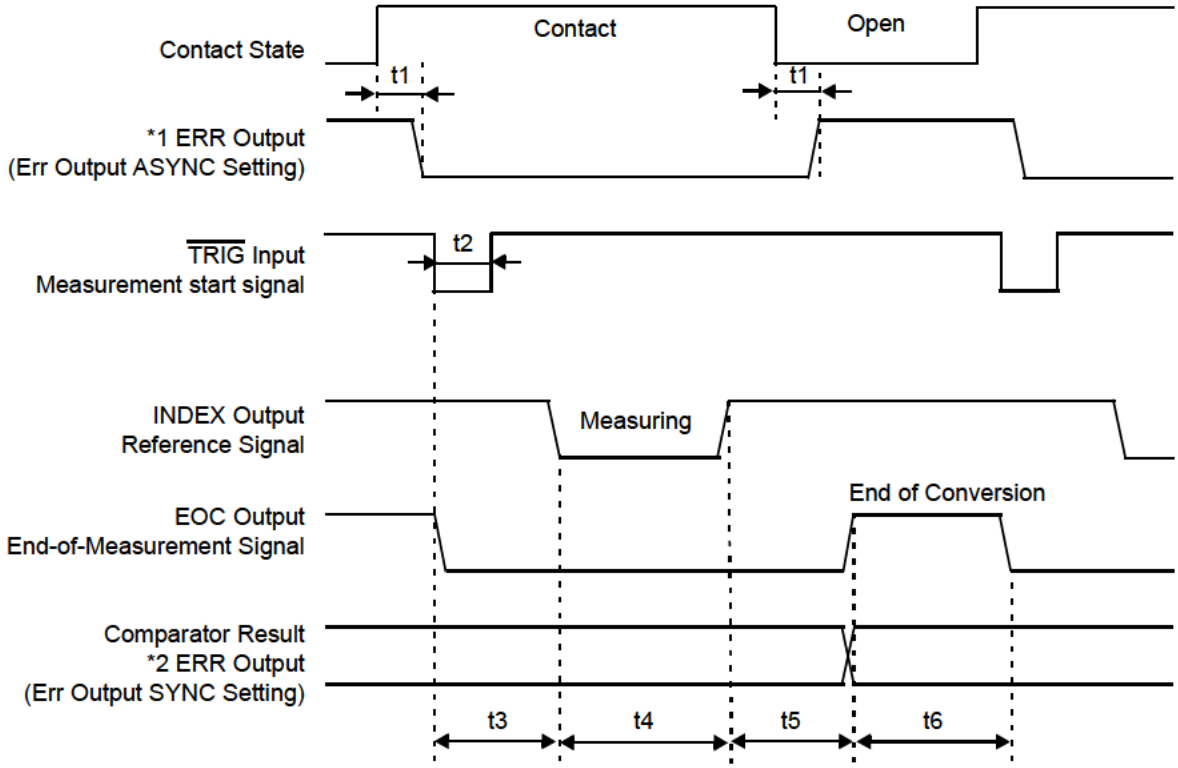

*1: For details, see "5.2.4 ERR Output (Page 73)."
*2: When ERR output is set to the SynChronous mode, measurement fault detection results can be obtained when measurement is finished, as with comparator results.

Internal Trigger Timing Chart

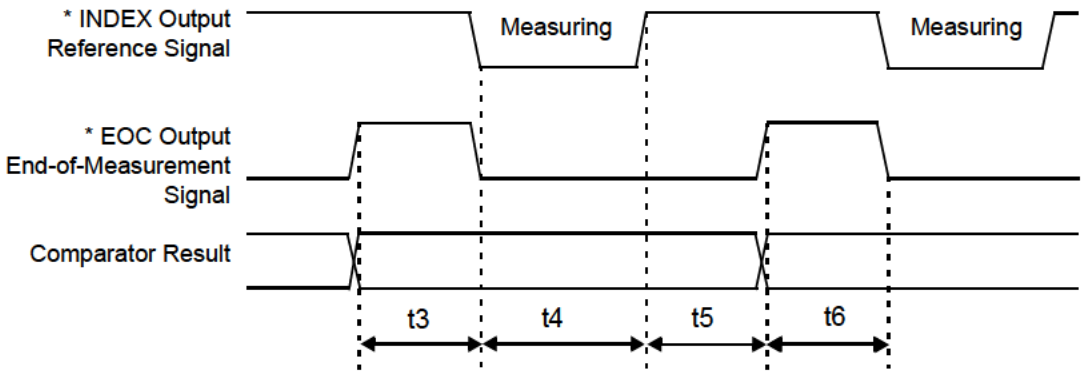

* When the EOC signal is set to PULSE, the signal will remain on only for the specified period upon completion of conversion.

Description		Time			
t1	ERR Output response time*1	1.5 ms			
t2	Measurement trigger pulse width	0.5 ms min.			
t3	Delay Time	per setting ❖See Section 4.2.2 Trigger Delay Settings (Page 52).			
t4	Measurement time*2	ΩV mode		Ω mode or V mode	
		EX.FAST	6.8 ms	EX.FAST	3.4 ms
		FAST	22.8 ms	FAST	11.4 ms
		MEDIUM	82.8 ms 68.8 ms	MEDIUM	41.4 ms (50 Hz line frequency setting) 34.4 ms (60 Hz line frequency setting)
		SLOW	257.8 ms 251.2 ms	SLOW	156.4 ms (50 Hz line frequency setting) 149.8 ms (60 Hz line frequency setting)
t5	Calculation time*3	0.3 ms			
t6	EOC Output pulse width	When the external trigger is selected HOLD setting : Holds until the next trigger is detected PULSE setting : Remains only for the specified pulse width ❖See Section 5.2.5 Instrument Settings (Page 74). When the internal trigger is selected HOLD setting : EX.FAST 1 ms, FAST 5 ms, MEDIUM 20 ms, SLOW 50 ms PULSE setting : Remains only for the specified pulse width			

*1: For details, see “5.2.4 ERR Output (Page 73).”

*2: About t4 measurement time

When averaging is enabled, the running average is obtained with internal triggering, so measurement time t4 does not change. The measurement time for external triggering is as follows:

With SLOW sampling

ΩV	(t4 - 57.8) X n + 57.8 ms (50 Hz)
	(t4 - 51.2) X n + 51.2 ms (60 Hz)
Ω or V	(t4 - 56.4) X n + 56.4 ms (50 Hz)
	(t4 - 49.8) X n + 49.8 ms (60 Hz)

With other than SLOW sampling

ΩV	(t4 - 2.8) X n + 2.8 ms
Ω or V	(t4 - 1.4) X n + 1.4 ms

(n represents the number of values averaged)

*3: About t5 calculation time

In the following cases, add the indicated times to calculation time t5:

When the Statistical Calculation function is enabled	0.3 ms
When the reference value/tolerance method of comparator decision is selected	0.15 ms

5.4 Internal Circuitry

External Control and External Output Terminal Ratings

	I/O type	Logic	Electrical specification
Output	Open collector		35 V DC, 50 mA DC max.
Input	C-MOS	Inverse logic	H: 3.8 to 5.0 V, L: 0 to 1.2 V

External Control Terminals

Circuit Diagram

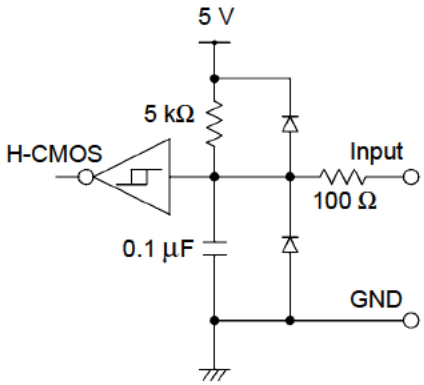

Application Examples

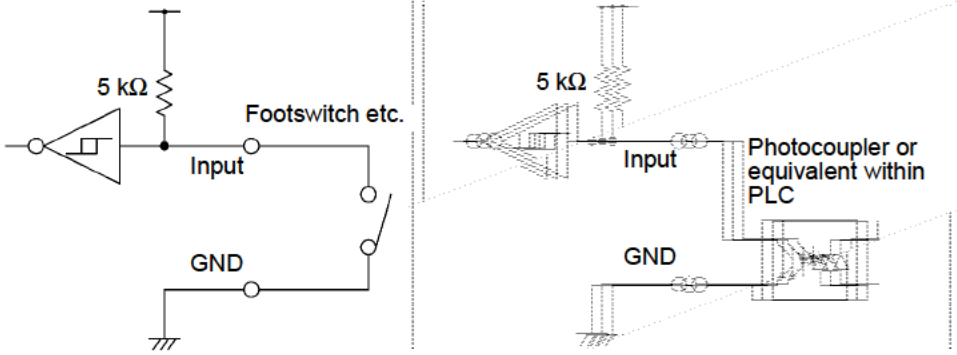

Switch Connection

Photocoupler Connection

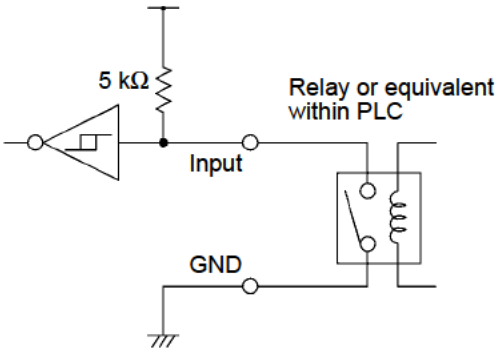

Relay Connection

External Output Terminals

Circuit Diagram

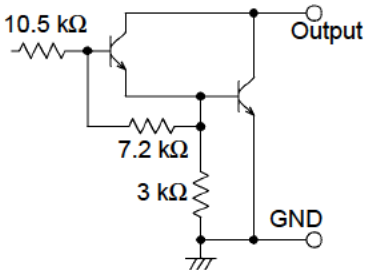

Open-Collector Output

Application Examples



Wired-OR

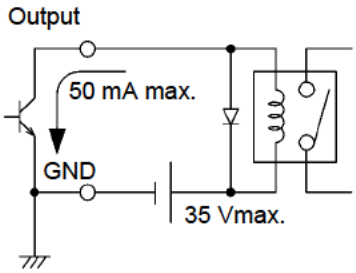

Relay Connection

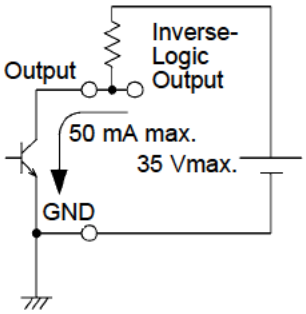

Inverse-Logic Output

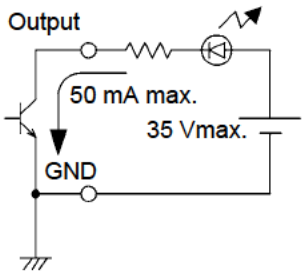

LED Connection

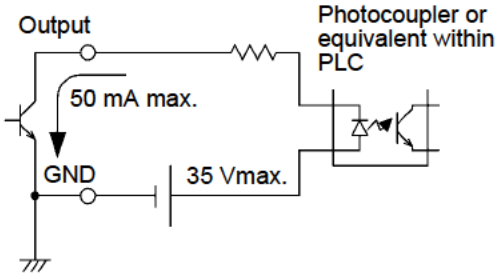

Photocoupler Connection

Chapter 6 Printer(Optional)

The following items can be printed using the optional Model 9670 PRINTER, 9638 RS-232C CABLE, 9671 AC ADAPTER and 9237 RECORDING PAPER:

- Measurement values and decision results
- Statistical calculation results

The following items are required to use the 9670 PRINTER.

- Model 9670 PRINTER (Sanei Electric Model BL-80RSII, supplied with a roll of thermal paper)
- Model 9671 AC ADAPTER (Sanei Electric Model BL-100W)
- Model 9237 RECORDING PAPER (thermal paper 80 x 25 m, 4 rolls)
- Model 9638 RS-232C CABLE

To use the printer with a battery:

- Model 9672 BATTERY PACK (Sanei Electric UR-100 or UR-121)
- Model 9673 BATTERY CHARGER (Sanei Electric NC-LSC01)

NOTE

- The 9670 PRINTER does not include a charging function for the 9672 BATTERY PACK. Use the 9673 BATTERY CHARGER to charge it.
- Read the manuals supplied with the printer and battery charger for the operating procedures.
- As much as possible, avoid printing in hot and humid environments. Otherwise, printer life may be severely shortened.
- Please use only the specified recording paper. Using non-specified paper may not only result in faulty printing, but printing may become impossible.
- If the recording paper is skewed on the roller, paper jams may result.
- Printing is not possible if the front and back of the recording paper are reversed.

6.1 Connecting the Printer

⚠WARNING

Because electric shock and instrument damage hazards are present, always follow the steps below when connecting the printer.

- **Always turn off the instrument and the printer before connecting.**
- **A serious hazard can occur if a wire becomes dislocated and contacts another conductor during operation. Make certain connections are secure.**

⚠CAUTION

If using a cable other than the 9638 RS-232C CABLE, the connector at the instrument end should be a molded type. The metal type (with hooks preventing the surface from being flat) will not fit due to the instrument's design.

NOTE

The requirements for a printer to be connected to the instrument are as follows.
Confirm compatibility and make the appropriate settings on the printer before connecting it to the instrument.

- Interface RS-232C
- Characters per line ..... At least 40
- Communication speed..... 9600 bps
- Data bits 8
- Parity ..... none
- Stop bits..... 1
- Flow control ..... none

6.1.1 Connecting the 9670 PRINTER to the Instrument

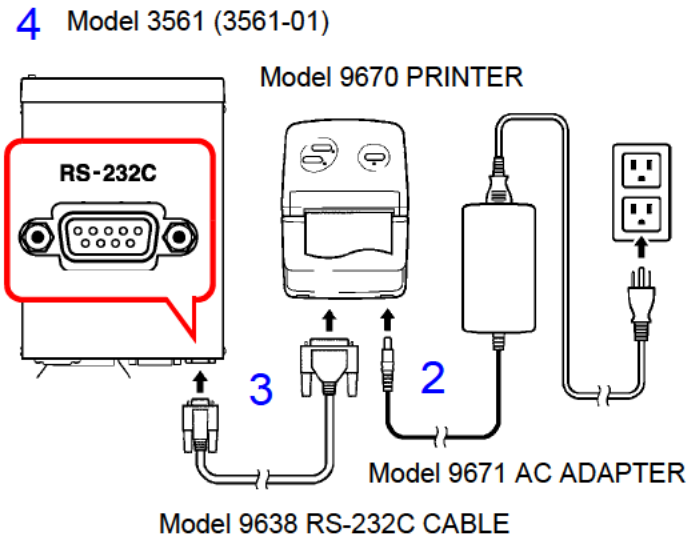

1. **Confirm that the instrument and 9670 PRINTER are turned off.**
2. **Connect the 9671 AC ADAPTER to the 9670 PRINTER, and insert the power plug into an outlet.**
3. **Connect the 9638 RS-232C CABLE to the RS-232C connectors on the instrument and printer.**
4. **Turn the instrument and printer on.**

For battery operation, use a fully charged Model 9672 BATTERY PACK.
❖See Section 6.1.3 Charging the Battery Pack (Page 83).

Connector Pinouts



Model 3561(-01) (9-pin) Connector

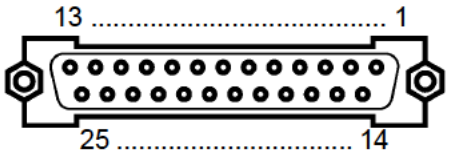

Model 9670 (25-pin) Connector

Function	Signal Name	Pin
Receive Data	RxD	2
Transmit Data	TxD	3
Signal or Common Ground	GND	5

Pin	Signal Name	Function
2	TxD	Transmit Data
3	RxD	Receive Data
7	GND	Signal or Common Ground
4	RTS	Request to Send
5	CTS	Clear to Send

6.1.2 Loading Recording Paper

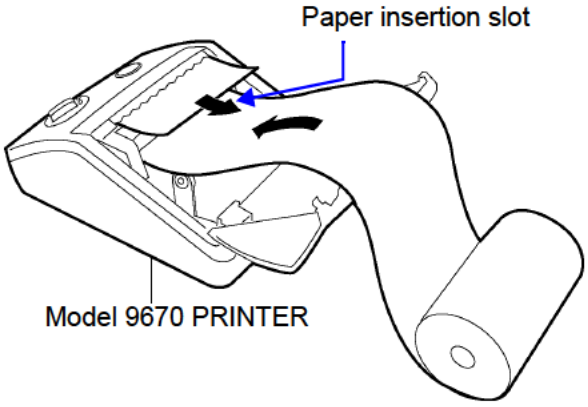

Load the recording paper into the 9670 PRINTER.

Note the paper orientation!





Cut the paper horizontally.

Handling and Storing Recording Paper

The recording paper is thermally and chemically sensitized. Observe the following precautions to avoid paper discoloration and fading.



Avoid exposure to direct sunlight.

Avoid exposure to volatile organic solvents like alcohol, ethers and ketones.

Do not store thermal paper above 40°C or 90% RH.

Avoid contact with adhesive tapes like soft vinyl chloride and cellophane tape.



Avoid stacking with wet Diazo copy paper.

NOTE

- Store thermal paper where its temperature will not exceed 40°C.
- The paper will deteriorate if exposed to light for a long time, so do not remove rolls from their wrappers until ready to use.
- Make photocopies of recording printouts that are to be handled or stored for legal purposes.

6.1.3 Charging the Battery Pack

1. **Plug the charger power cord into an outlet.**
2. **Insert the battery pack by sliding it in the direction indicated by the arrow.**

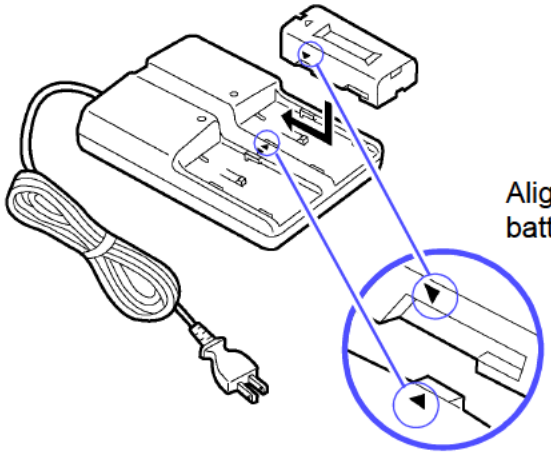

6.1.4 Installing the Battery Pack in the Printer

1. **Remove the battery compartment cover by sliding it in the direction indicated by the arrow.**
2. **Install the battery pack with its arrow pointing as shown at the left.**

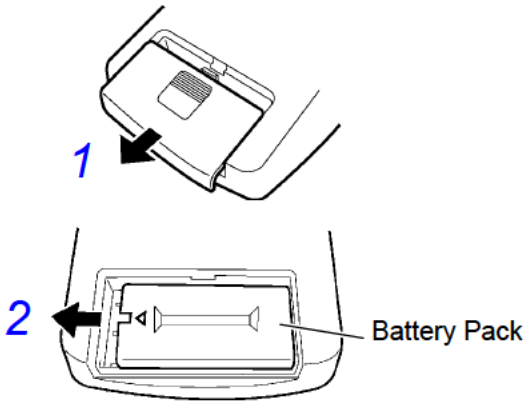

6.2 Selecting the Interface

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

Select the Interface Selection display.
❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).

(Main Display)

(Sub Display)
The current setting blinks.

Select Printer on the Sub Display.
rS..... RS-232C
GP-Ib.... GP-IB
Prn ..... Printer

3 Or ten-keys

Set the print interval time.
0000 .....Interval printing is OFF. (Printing is carried out once when **PRINT** key is pressed.)
0001 to 3600 .....Sets the print interval time in seconds.

4 ENTER

Applies setting and returns to the Measurement display.

6.3 Setting of the 9670 PRINTER

Turn the 9670 PRINTER on while holding the **FEED** button.
Then press **SELECT** to set as needed according to print results.
Model 9670 can be used with factory default settings.
The settings are as follows:

International char = Japan
Print mode = Graphic
Character set = 24Dot ANK Gothic type
Select switch = Available (ON)
Baud rate = 9600 bps
Bit length = 8bit
Parity = Non
Data control = SBUSY
Paper selection = Normal paper
Upright/inverted = Upright printing
Auto power off = Available (ON) [as needed]
Battery mode = Invalidity (OFF) [as needed]

6.4 Printing

Printing Measured Values and Decision Results

From the Measurement display, press the **PRINT** key or ground the $\overline{\text{PRINT}}$ pin in the EXT I/O connector to print the measured value and decision result.

NOTE

- When using the external trigger, if you want to print after a triggered measurement finishes, connect the EOC signal of the EXT I/O to the $\overline{\text{PRINT}}$ signal.
- To print all measurements continuously, connect the EOC signal to the $\overline{\text{PRINT}}$ signal and enable the internal trigger.
- When the statistical calculation function is on and the internal trigger is selected, the **TRIG** key or $\overline{\text{TRIG}}$ signal will trigger statistical calculation and printing of the current measurement value.
- Valid counts are 1 to 30000. Above 30000, the count returns to 1.

Interval Printing

This function allows you to automatically print out measurement results at preset intervals. The print interval time must be set from the Interface Selection display.
❖See Section 6.2 Selecting the Interface (Page 84).
The setting range is 1 to 3600 seconds.
When the print interval time is set to "0", interval printing is disabled, and only normal printing is carried out.

Operation when interval printing is selected:

1. Start printing by pressing the **PRINT** key or sending the $\overline{\text{PRINT}}$ signal via EXT I/O.
2. Elapsed time (hours/minutes/seconds) and measurement values are printed automatically at intervals corresponding to the preset interval time.
3. Stop printing by pressing the **PRINT** key or sending the $\overline{\text{PRINT}}$ signal via EXT I/O again.

NOTE

- When the printed elapsed time reaches 100 hours, it resets to 00:00:00 and continues from zero.
  (Example)
  After 99 hours, 59 minutes and 50 seconds: 99:59:50
  After 100 hours, 2 minutes and 30 seconds: 00:02:30
- Selecting a display other than the measurement display causes interval printing to stop.

Printing Statistical Calculation Results

From the Statistical Calculation display, press the **PRINT** key to print statistical calculation results. If no valid data exists, only the data count is printed. When only one valid data sample exists, standard deviation of sample and process capability indices cannot be printed.

Example Printouts

Measurement values (ΩV mode)

```
  1    298.60mOhm,   1.3924 V
  2    0.2984 Ohm,   1.3924 V
  3 -    3.35mOhm,   0.0000 V
  4 - 0.0054 Ohm,    0.0000 V
  5    299.10mOhm,- 1.3923 V
  6    0.2984 Ohm,- 1.3923 V
  7      3.57mOhm, 13.9071 V
  8 -   16.89mOhm,-13.9088 V
```

Measurement values (Ω mode)

```
 15    209.98mOhm
 16    0.2103 Ohm
```

Measurement values (V mode)

```
3132    4.2019 V
3133   15.2084 V
```

With the Comparator ON

```
 95    105.80mOhm Lo,   0.0000 V    IN
 96    213.15mOhm Hi
 97    213.12mOhm IN
 98    213.11mOhm Lo
 99   10.0072 V    Hi
100   10.0071 V    IN
101   10.0070 V    Lo
102     O.F.       Hi,    O.F.       Hi
103 -    3.11mOhm Lo,-   O.F.       Lo
104 --------       --,--------      --
```

With the relative value comparison method (reference value and tolerance)

```
 84     0.023 %    Hi,    0.001 %    IN
 85     0.014 %    IN,    0.000 %    IN
 86 -   0.019 %    Lo,    0.002 %    IN
```

With erroneous measurement values

```
 10     O.F.       ,    O.F.
 11 -   O.F.       ,-   O.F.
 12 --------       ,--------
 13   Invalid      , Invalid
 14     O.F.       , 12.0097 V
 15 -   19.82mOhm,-   O.F.
```

Statistical Calculations (Comparator ON)

Max/Min count

```
*** RESISTANCE ***
Number          85
Valid           85
Average     13.06mOhm
Max         13.78mOhm(     74)
Min         12.10mOhm(      3)
Sn           0.38mOhm
Sn-1         0.38mOhm
Cp           1.32
CpK          0.09
Comp Hi        40
Comp IN        45
Comp Lo         0


***   VOLTAGE    ***
Number          85
Valid           85
Average   10.0074 V
Max       10.0197 V   (     57)
Min        9.9938 V   (     31)
Sn         0.0068 V
Sn-1       0.0068 V
Cp           0.35
CpK          0.32
Comp Hi        10
Comp IN        59
Comp Lo        16
```

Interval print

```
00:00:00    13.74mOhm, 10.0138 V
00:00:01    13.87mOhm, 10.0138 V
00:00:02    13.67mOhm, 10.0139 V
00:00:03    13.47mOhm, 10.0138 V
00:00:04    13.58mOhm, 10.0139 V
00:00:05    13.58mOhm, 10.0139 V
00:00:06    13.68mOhm, 10.0139 V
```

NOTE

Measurement values indicated as "Invalid" cannot be displayed by the instrument.
The number of statistical calculation results indicated as “Valid” equals the count of valid data excluding measurement faults and overflows.

RS-232C/GP-IB Interfaces Chapter 7

This chapter describes the GP-IB and RS-232C interfaces, using the following symbols to indicate which information pertains to each interface. Sections with neither of these symbols pertain to both interfaces.

GP-IB : GP-IB only

RS-232C : RS-232C only

Before Use

- GP-IB is available only on Model 3561-01.
- Always make use of the connector screws to affix the GP-IB or RS-232C connectors.
- When issuing commands that contain data, make certain that the data is provided in the specified format.

7.1 Overview and Features

All instrument functions other than power on/off switching can be controlled via GP-IB/RS-232C interfaces.

- Resetting is supported.

GP-IB

- IEEE 488.2-1987 Common (essential) Commands are supported.
- Complies with the following standard:
  Applicable standard IEEE 488.1-1987*1
- This instrument is designed with reference to the following standard:
  Reference standard IEEE 488.2-1987*2
- If the output queue becomes full, a query error is generated and the output queue is cleared. Therefore, clearing the output queue and query error output from the deadlocked condition*3 as defined in IEEE 488.2 is not supported.

*1. ANSI/IEEE Standard 488.1-1987, IEEE Standard Digital Interface for Programmable Instrumentation.

*2. ANSI/IEEE Standard 488.2-1987, IEEE Standard Codes, Formats, Protocols, and Common Commands.

*3. The situation in which the input buffer and the output queue become full, so that processing cannot continue.

7.2 Specifications

7.2.1 RS-232C Specifications

RS-232C

Transfer method	Communications : Full duplex Synchronization : Start-stop synchronization
Baud rate	9600 bps/ 19200 bps/ 38400 bps
Data length	8 bit
Parity	none
Stop bit	1 bit
Message terminator (delimiter)	Receiving : CR+LF, CR Transmitting : CR+LF
Flow control	none
Electrical specification	Input voltage levels 5 to 15 V: ON, -15 to -5 V: OFF Output voltage levels 5 to 9 V: ON, -9 to -5 V: OFF
Connector	RS-232C Interface Connector Pinout (Male 9-pin D-sub, with #4-40 attachment screws) The I/O connector is a DTE (Data Terminal Equipment) configuration Recommended cables: • Model 9637 RS-232C CABLE (for PC/AT-compatibles) • Model 9638 RS-232C CABLE (for PC98-series) ❖See Section 7.3.1 Attaching the Connector (Page 89).

7.2.2 GP-IB Specifications (Model 3561-01 only)

GP-IB is available only on Model 3561-01.

GP-IB

Interface Functions

SH1	All Source Handshake functions are supported.
AH1	All Acceptor Handshake functions are supported.
T6	Basic talker functions are supported. Serial poll function are supported. No talk-only mode. The talker cancel function with MLA (My Listen Address) is supported.
L4	Basic listener functions are supported. No listen-only mode. The listener cancel function with MTA (My Talk Address) is supported.
SR1	All Service Request functions are supported.
RL1	All Remote/Local functions are supported.
PP0	No Parallel Poll function.
DC1	All Device Clear functions are supported.
DT1	All Device Trigger functions are supported.
C0	No Controller functions are supported.

Operating Code: ASCII codes

7.3 Selecting the Connections and Protocol

7.3.1 Attaching the Connector

WARNING

- **Always turn both devices OFF when connecting and disconnecting an interface connector. Otherwise, an electric shock accident may occur.**
- **After connecting, always tighten the connector screws. The mounting screws must be firmly tightened or the RS-232C connector may not perform to specifications, or may even fail.**
- **To avoid damage to the instrument, do not short-circuit the connector and do not input voltage to the connector.**

RS-232C

RS-232C Connector



Male 9-pin D-sub
#4-40 attaching screws

Connect the RS-232C cable.

To connect the instrument to a controller (DTE), use a crossover cable compatible with the connectors on both the instrument and the controller.

The I/O connector is a DTE (Data Terminal Equipment) configuration. This instrument uses only pins 2, 3 and 5. The other pins are unconnected.

Pin No.	Signal Name			Signal	Notes
	Common	EIA	JIS		
1	DCD	CF	CD	Unused	No connection
2	RxD	BB	RD	Receive Data	
3	TxD	BA	SD	Transmit Data	
4	DTR	CD	ER	Data Terminal Ready	Internally connected to +5 V
5	GND	AB	SG	Signal Ground	
6	DSR	CC	DR	Unused	No connection
7	RTS	CA	RS	Request to Send	Internally connected to +5 V
8	CTS	CB	CS	Unused	No connection
9	RI	CE	CI	Unused	No connection

RS-232C

Connecting to a PC/AT-Compatible (DOS/V) Machine

Use a **crossover cable** with **female 9-pin D-sub** connectors.

Crossover Wiring

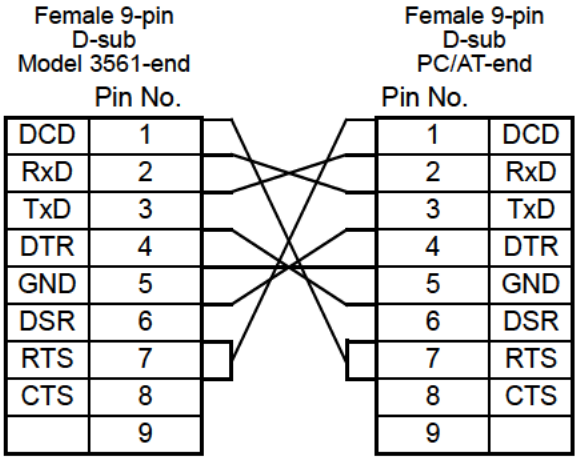

Recommended cable:

HIOKI
Model 9637 RS-232C CABLE (1.8 m)

Connecting to an NEC PC9801 or PC9821 Series Desktop PC (excluding NX)

Use a **crossover cable** with **a female 9-pin D-sub** and **a male 25-pin D-sub** connector.
As the figure shows, RTS and CTS pins are shorted together and crossed to DCD in the other connector.

Crossover Wiring

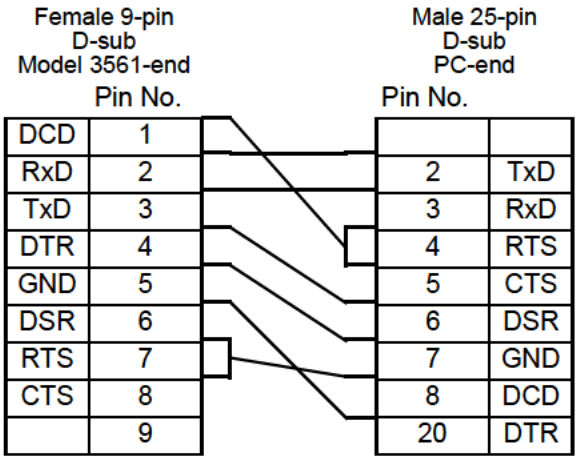

Recommended cable:

HIOKI
Model 9638 RS-232C CABLE (1.8 m)

Note that the combination of a dual male 25-pin D-sub cable and a 9- to 25-pin adapter cannot be used.

GP-IB

GP-IB Connector



Connecting a GP-IB cable.

Recommended cable:
Model 9151-02 GP-IB CONNECTOR CABLE (2 m)
Model 9151-04 GP-IB CONNECTOR CABLE (4 m)

7.3.2 Selecting the Interface

1 SHIFT → ENTER (MENU)

(SHIFT Lamp lit)

The Menu display appears.

2

Select the Interface Selection display.

❖See Section 1.4 Menu Display Sequence (SHIFT → ENTER) (Page 13).



(Main Display)

(Sub Display)
The current setting blinks.

3

Select RS-232C or GP-IB on the Sub Display.

rS RS-232C
GP-Ib .... GP-IB (Model 3561-01 only)
Prn ..... Printer

When you select RS-232C, set the communications speed.

(Sub Display)

When selecting **GP-IB**, also set the Address and Message Terminator.

(Sub Display)

Message Terminator setting (LF/CRLF)

Address setting (0 to 30)

Selects the item to set

Setting

4 ENTER

Applies settings and returns to the Measurement display.

7.4 Communication Methods

Various messages are supported for controlling the instrument through the interfaces.
Messages can be either program messages, sent from the PC to the instrument, or response messages, sent from the instrument to the PC.

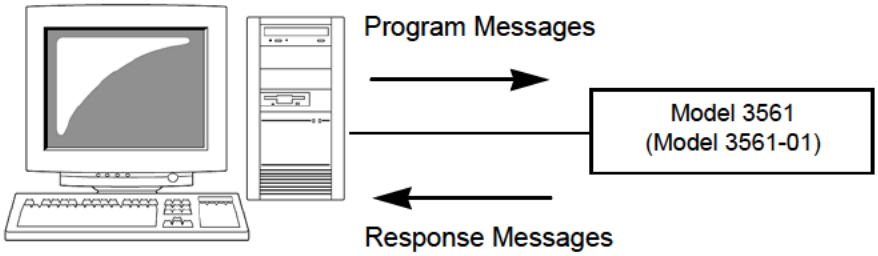

Message types are further categorized as follows:

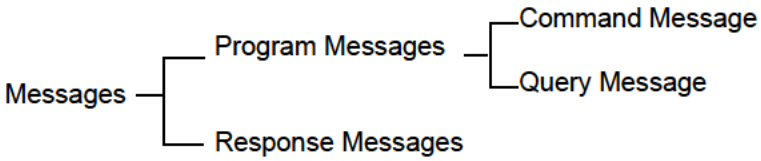

7.4.1 Message Format

Program Messages

Program messages can be either Command Messages or Query Messages.

- **Command Messages**
  Instructions to control the instrument, such as to change settings or reset

  Example: (instruction to set the measurement range)

  ```
  :RESISTANCE:RANGE 100E-3
  ```

  Header portion — Space — Data portion

- **Query Messages**
  Requests for responses relating to results of operation or measurement, or the state of instrument settings.

  Example: (request for the current measurement range)

  ```
  :RESISTANCE:RANGE?
  ```

  Header portion — Question Mark

❖For details: See Section Headers (Page 93), Separators (Page 94) and Data Formats (Page 95).

Response Messages

When a query message is received, its syntax is checked and a response message is generated.
The :SYSTem:HEADer command determines whether headers are prefixed to response messages.

Header ON :RESISTANCE:RANGE 300.00E-3
Header OFF 300.00E-3
(the current resistance measurement range is 300 mΩ)

At power-on, Header OFF is selected.
If an error occurs when a query message is received, no response message is generated for that query.
No header is applied to commands used only for queries, such as :FETCH? and :CALCulate:LIMit:RESistance:RESult?.

Command Syntax

Command names are chosen to mnemonically represent their function, and can be abbreviated. The full command name is called the "long form", and the abbreviated name is called the "short form".
The command references in this manual indicate the short form in upper-case letters, extended to the long form in lower case letters, although the commands are not case-sensitive in actual usage.
Response messages generated by the instrument are in long form and

FUNCTION	OK (long form)
FUNC	OK (short form)
FUNCT	Error
FUN	Error

in upper case letters.

Headers

Headers must always be prefixed to program messages.

(1) Command Program Headers

There are three types of commands: Simple, Compound and Standard.

- **Headers for Simple Commands**
  This header type is a sequence of letters and digits
  *ESE 0
- **Headers for Compound Commands**
  These headers consist of multiple simple command type headers separated by colons ":"
  :SAMPle:RATE
- **Headers for Standard Commands**
  This header type begins with an asterisk "*",
  indicating that it is a standard command defined by IEEE 488.2.
  *RST

(2) Query Program Header

These commands are used to interrogate the instrument about the results of operations, measured values and the current states of instrument settings.
As shown by the following examples, a query is formed by appending a question mark "?" after a program header.

:FETCh?
:MEASure:RESistance?

Message Terminators

This instrument recognizes the following message terminators:

GP-IB
- LF
- CR+LF
- EOI
- LF with EOI

RS-232C
- CR
- CR+LF

From the instrument's interface settings, the following can be selected as the terminator for response messages.

GP-IB
- LF with EOI (initial setting)
- LF with CR and EOI

RS-232C
- CR + LF (initial setting)

❖See Section 7.3.2 Selecting the Interface (Page 91).

Separators

(1) Message Unit Separator

Multiple message can be written in one line by separating them with semicolons ";".

```
:SYSTEM:LFREQUENCY 60;*IDN?
```

- When messages are combined in this way and if one command contains an error, all subsequent messages up to the next terminator will be ignored.
- A query error occurs if a query command is combined with an immediately following semicolon and subsequent command.

(2) Header Separator

In a message consisting of both a header and data, the header is separated from the data by a space " ".

```
:SYSTEM:ELOCK ON
```

(3) Data Separator

In a message containing multiple data items, commas are required to separate the data items from one another.

Data Formats

The instrument uses character data and decimal numeric data, depending on the command.

(1) Character Data

Character data always begins with an alphabetic character, and subsequent characters may be either alphabetic or numeric. Character data is not case-sensitive, although response messages from the instrument are only upper case.
As with command syntax, both long and short forms are acceptable.

```
:SYSTEM:ELOCK ON
```

(2) Decimal Numeric Data

Three formats are used for numeric data, identified as NR1, NR2 and NR3. Numeric values may be signed or unsigned. Unsigned numeric values are handled as positive values.
Values exceeding the precision handled by the instrument are rounded to the nearest valid digit.

- NR1 Integer data (e.g.: +12, -23, 34)
- NR2 Fixed-point data(e.g.: +1.23, -23.45, 3.456)
- NR3 Floating-point exponential representation data
  (e.g.: +1.0E-2, -2.3E+4)

The term "NRf format" includes all three of the above numeric decimal formats.
The instrument accepts NRf format data.

The format of response data is specified for each command, and the data is sent in that format.

```
:ESR0 106
:FETCH? +106.57E-3
```

GP-IB

The instrument does not fully support IEEE 488.2. As much as possible, please use the data formats shown in the Reference section. Also, be careful to avoid constructing single commands that could overflow the input buffer or output queue.

Compound Command Header Omission

When several commands having a common header are combined to form a compound command (e.g., `:CALCulate: LIMit:RESistance:UPPer:` and `:CALCulate:LIMit:RESistance:LOWer`), if they are written together in sequence, the common portion (here, `:CALCulate:LIMit:RESistance`) can be omitted after its initial occurrence.
This common portion is called the "current path" (analogous to the path concept in computer file storage), and until it is cleared, the interpretation of subsequent commands presumes that they share the same common portion.

This usage of the current path is shown in the following example:

Full expression

```
:CALCulate:LIMit:RESistance:UPPer
30000;:CALCulate:LIMit:LOWer 29000
```

Compacted expression

```
:CALCulate:LIMit:RESistance:UPPer 30000;LOWer 29000
```

This portion becomes the current path, and can be omitted from the messages immediately following.

The current path is cleared when the power is turned on, when reset by key input, by a colon "`:`" at the start of a command, and when a message terminator is detected.
Standard command messages can be executed regardless of the current path.
They have no effect upon the current path.

A colon "`:`" is not required at the start of the header of a Simple or Compound command. However, to avoid confusion with abbreviated forms and operating mistakes, we recommend always placing a colon at the start of a header.

7.4.2 Output Queue and Input Buffer

Output Queue

Response messages are stored in the output queue until read by the controller. The output queue is also cleared in the following circumstances:

- Power on
- Device clear
- Query Error

The output queue capacity of the instrument is 64 bytes. If response messages overflow the buffer, a query error is generated and the output queue is cleared.
Also, with GP-IB, if a new message is received while data remains in the output queue, the output queue is cleared and a query error is generated.

Input Buffer

The input buffer capacity of the instrument is 256 bytes.
If 256 bytes are allowed to accumulate in this buffer so that it becomes full, the GP-IB interface bus enters the waiting state until space is cleared in the buffer.
The RS-232C interface will not accept data beyond 256 bytes.

NOTE Ensure that the no command ever exceeds 256 bytes.

7.4.3 Status Byte Register

This instrument implements the status model defined by IEEE 488.2 with regard to the serial poll function using the service request line.
The term "event" refers to any occurrence that generates a service request.

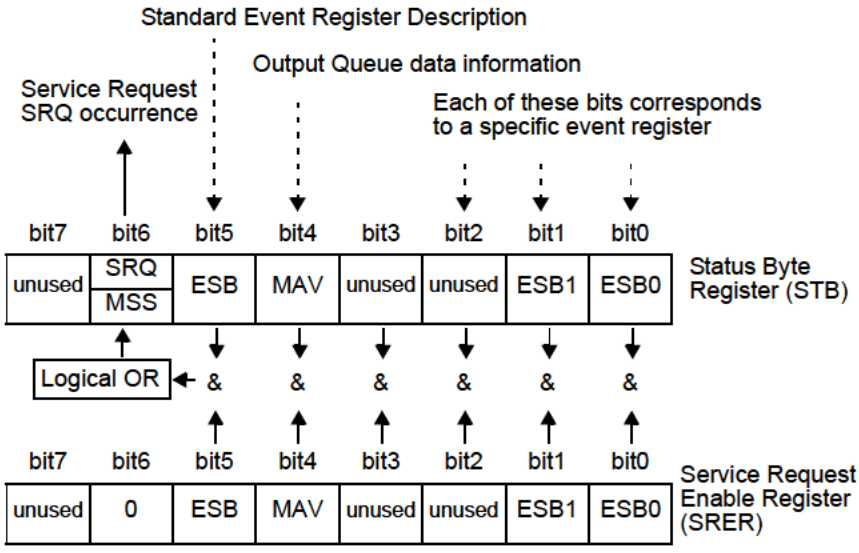

Overview of Service Request Occurrence

The Status Byte Register contains information about the event registers and the output queue. Required items are selected from this information by masking with the Service Request Enable Register. When any bit selected by the mask is set, bit 6 (MSS; the Master Summary Status) of the Status Byte Register is also set, which generates an SRQ (Service Request) message and dispatches a service request.

Status Byte Register (STB)

During serial polling, the contents of the 8-bit Status Byte Register are sent from the instrument to the controller.
When any Status Byte Register bit enabled by the Service Request Enable Register has switched from 0 to 1, the MSS bit becomes 1. Consequently, the SRQ bit is set to 1, and a service request is dispatched.

The SRQ bit is always synchronous with service requests, and is read and simultaneously cleared during serial polling. Although the MSS bit is only read by an `*STB?` query, it is not cleared until a clear event is initiated by the `*CLS` command.

Bit 7	unused
Bit 6 SRQ MSS	Set to 1 when a service request is dispatched. This is the logical sum of the other bits of the Status Byte Register.
Bit 5 ESB	Standard Event Status (logical OR) bit This is logical sum of the Standard Event Status Register.
Bit 4 MAV	Message available Indicates that a message is present in the output queue.
Bit 3	unused
Bit 2	unused
Bit 1 ESB1	Event Status (logical OR) bit 1 This is the logical sum of Event Status Register 1.
Bit 0 ESB0	Event Status (logical OR) bit 0 This is the logical sum of Event Status Register 0.

Service Request Enable Register (SRER)

This register masks the Status Byte Register. Setting a bit of this register to 1 enables the corresponding bit of the Status Byte Register to be used.

7.4.4 Event Registers

Standard Event Status Register (SESR)

The Standard Event Status Register is an 8-bit register.
If any bit in the Standard Event Status Register is set to 1 (after masking by the Standard Event Status Enable Register), bit 5 (ESB) of the Status Byte Register is set to 1.

The Standard Event Status Register is cleared in the following situations:

- When a ***CLS** command is executed
- When an event register query (***ESR?**) is executed
- When the instrument is powered on

Bit 7	PON	Power-On Flag Set to 1 when the power is turned on, or upon recovery from an outage.
Bit 6		User Request unused
Bit 5	CME	Command Error (The command to the message terminator is ignored.) This bit is set to 1 when a received command contains a syntactic or semantic error: • Program header error • Incorrect number of data parameters • Invalid parameter format • Received a command not supported by the instrument
Bit 4	EXE	Execution Error This bit is set to 1 when a received command cannot be executed for some reason. • The specified data value is outside of the set range • The specified setting data cannot be set • Execution is prevented by some other operation being performed
Bit 3	DDE	Device-Dependent Error This bit is set to 1 when a command cannot be executed due to some reason other than a command error, a query error or an execution error. • Execution is impossible due to an internal instrument fault
Bit 2	QYE	Query Error (the output queue is cleared) This bit is set to 1 when a query error is detected by the output queue control. • When an attempt has been made to read an empty output queue (GP-IB only) • When the data overflows the output queue • When data in the output queue has been lost
Bit 1		unused
Bit 0	OPC	Operation Complete (GP-IB only) This bit is set to 1 in response to an ***OPC** command. • It indicates the completion of operations of all messages up to the ***OPC** command

Standard Event Status Enable Register (SESER)

Setting any bit of the Standard Event Status Enable Register to 1 enables access to the corresponding bit of the Standard Event Status Register.

Standard Event Status Register (SESR) and Standard Event Status Enable Register (SESER)

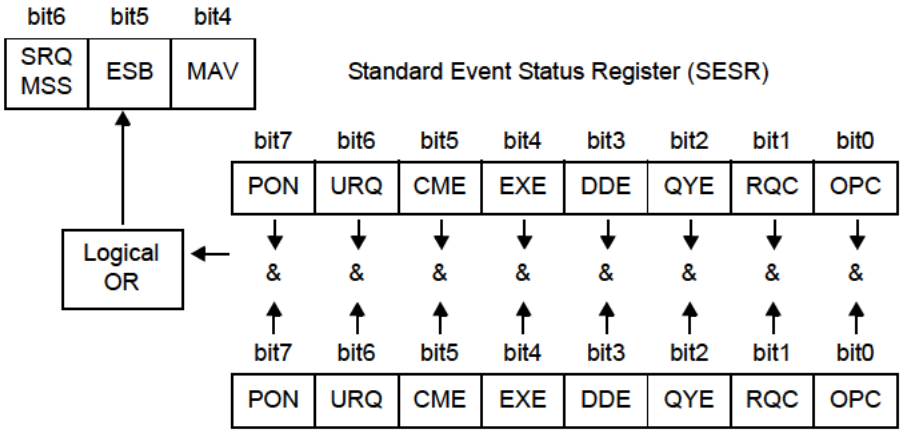

Standard Event Status Enable Register (SESER)

Device-Specific Event Status Registers (ESR0 and ESR1)

This instrument provides two event status registers for controlling events.

Each event register is an 8-bit register.

When any bit in one of these event status registers enabled by its corresponding event status enable register is set to 1, the following happens:

- For Event Status Register 0, bit 0 (ESB0) of the Status Byte Register is set to 1.
- For Event Status Register 1, bit 1 (ESB1) of the Status Byte Register is set to 1.

Event Status Registers 0 and 1 are cleared in the following situations:

- When a **`*CLS`** command is executed
- When an Event Status Register query (**`:ESR0?`** or **`:ESR1?`**) is executed
- When the instrument is powered on

	Event Status Register 0 (ESR0)		Event Status Register 1 (ESR1)	
Bit 7	--	Unused	--	unused
Bit 6	--	Unused	AND	AND
Bit 5	ERR	Measurement Faults	V-Hi	Voltage High Comparator Result
Bit 4	--	Unused	V-IN	Voltage IN Comparator Result
Bit 3	--	Unused	V-Lo	Voltage Low Comparator Result
Bit 2	--	Unused	R-Hi	Resistance High Comparator Result
Bit 1	INDEX	End of Measurement	R-IN	Resistance IN Comparator Result
Bit 0	EOC	End of Conversion	R-Lo	Resistance Low Comparator Result

Event Status Registers 0 (ESR0) and 1 (ESR1), and Event Status Enable Registers 0 (ESER0) and 1 (ESER1)

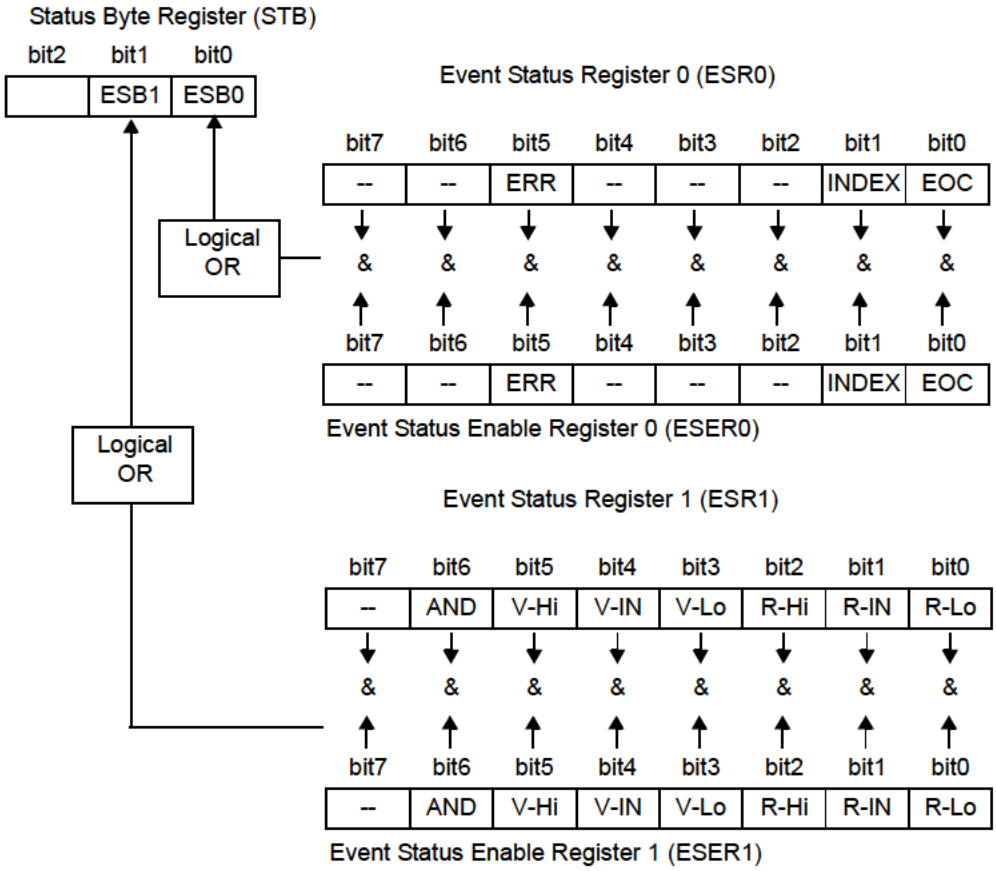

Register Reading and Writing

Register	Read	Write
Status Byte Register	*STB?	–
Service Request Enable Register	*SRE?	*SRE
Standard Event Status Register	*ESR?	–
Standard Event Status Enable Register	*ESE?	*ESE
Event Status Register 0	:ESR0?	–
Event Status Enable Register 0	:ESE0?	:ESE0
Event Status Register 1	:ESR1?	–
Event Status Enable Register 1	:ESE1?	:ESE1

GP-IB Commands

The following commands can be used for performing interface functions.

Command	Description	
GTL	Go To Local	Cancels the Remote state and enters the Local state.
LLO	Local Lock Out	Disables all keys, including the **LOCAL** key.
DCL	Device CLear	Clears the input buffer and the output queue.
SDC	Selected Device Clear	Clears the input buffer and the output queue.
GET	Group Execute Trigger	When an external trigger occurs, processes one sample.

7.4.5 Initialization Items

● = initialized, — = not initialized

Item \ Initialization Method	At Power-on	*RST Command	Device Clear	*CLS Command
Device-specific functions (Range, etc.)	—	●	—	—
Output Queue	●	—	●	—
Input buffer	●	—	●	—
Status Byte Register	●	—	—*1	●*2
Event registers	●*3	—	—	●
Enable register	●	—	—	—
Current path	●	—	●	—
Headers on/off	●	●	—	—

*1: Only the MAV bit (bit 4) is cleared.
*2: All bits except the MAV bit are cleared.
*3: Except the PON bit (bit 7).

7.4.6 Local Function

During communications, **REMOTE** is lit to indicate the remote control state.

To cancel the Remote state

LOCAL REMOTE off

NOTE

- Remote control can be canceled by pressing the **SHIFT** key and then the **AUTO** key.
- If the Local Lock Out (Page 102) GP-IB command has been issued, the Remote state cannot be canceled.

7.5 Message List

Commands specific to RS-232C or GP-IB are identified by RS-232C or GP-IB, respectively.

NOTE

- Any spelling mistake in a message results in a command error.
- < > = contents of the data portion.
  [Numeric data values are indicated by format as (NR1), (NR2) and (NR3), representing integer, fixed-point and floating point decimal data values respectively, or as (NRf), representing any of these formats]
- [ ]: optional

7.5.1 Standard Commands

Command	Data Formats (Response data if a Query)	Description	Error	Ref page
∗IDN?	<Manufacturer's name>, <Model name>,0, <Software version>	Queries the device ID	*2	111
∗RST		Initializes the device	*1	111
∗TST?	0 to 3 (NR1)	Initiates a self-test and queries the result	*2	111
∗OPC		Requests an SRQ after execution completion	*1	112
∗OPC?	1	Queries execution completion	*2	112
∗WAI		Waits for operations to finish	*1	112
∗CLS		Clears the Event Registers and the Status Byte Register	*1	112
∗ESE	0 to 255 (NR1)	Sets the contents of the Standard Event Status Enable Register	*3	113
∗ESE?	0 to 255 (NR1)	Queries the Standard Event Status Enable Register	*2	113
∗ESR?	0 to 255 (NR1)	Queries and clear the Standard Event Status Register	*2	113
∗SRE	0 to 255 (NR1)	Sets the Service Request Enable Register	*3	114
∗SRE?	0 to 255 (NR1)	Queries the contents of the Service Request Enable Register	*2	114
∗STB?	0 to 255 (NR1)	Queries the Status Byte Register	*2	114
∗TRG		Requests a sampling	*1	114

Error description (an error occurs when executing messages in the following cases):

*1 Command Error.....When data is present after the command
*2 Query Error.....When the response message exceeds 64 bytes
*3 Execution Error.....When invalid character or numeric data is present

7.5.2 Device-Specific Commands

Message ([ ] = optional)	Data Contents ( ) = response data	Description	Ref page
Event Registers			
:ESE0	0 to 255	Sets Event Status Enable Register 0	115
:ESE0?	0 to 255	Queries Event Status Enable Register 0	115
:ESR0?	0 to 255	Queries Event Status Register 0	115
:ESE1	0 to 255	Sets Event Status Enable Register 1	115
:ESE1?	0 to 255	Queries Event Status Enable Register 1	115
:ESR1?	0 to 255	Queries Event Status Register 1	115
Measurement Mode			
:FUNCtion	RV/ RESistance/ VOLTage	Sets measurement mode	116
:FUNCtion?	RV/ RESistance/ VOLTage	Queries measurement mode	116
Measurement Range			
:RESistance:RANGe	0 to 3.1	Sets resistance measurement range	116
:RESistance:RANGe?	300.00E-3/ 3.0000E+0	Queries resistance measurement range	116
:VOLTage:RANGe	-20 to 20	Sets voltage measurement range	116
:VOLTage:RANGe?	20.0000E+0	Queries voltage measurement range	116
Auto Range			
:AUTorange	1/ 0/ ON/ OFF	Sets the auto range	117
:AUTorange?	ON/ OFF	Queries the auto range setting	117
Zero-Adjust			
:ADJust:CLEAr		Cancels zero-adjustment	117
:ADJust?	0/ 1	Executes zero-adjustment and queries the result	117
Sampling Rate			
:SAMPle:RATE	EXFast/ FAST/ MEDium/ SLOW	Sets the sampling rate	117
:SAMPle:RATE?	EXFast/ FAST/ MEDium/ SLOW	Queries the sampling rate setting	117
Averaging Function			
:CALCulate:AVERage:STATe	1/ 0/ ON/ OFF	Sets averaging function execution	118
:CALCulate:AVERage:STATe?	ON/ OFF	Queries the averaging function execution setting	118
:CALCulate:AVERage	2 to 16	Sets the no. of samples to average	118
:CALCulate:AVERage?	2 to 16	Queries the no. of samples to average setting	118
Comparator			
:CALCulate:LIMit:STATe	1/ 0/ ON/ OFF	Sets comparator execution	118
:CALCulate:LIMit:STATe?	ON/OFF	Queries the comparator execution setting	118

Message ([ ] = optional)	Data Contents ( ) = response data	Description	Ref page
Comparator			
:CALCulate:LIMit:BEEPer	OFF/ HL/ IN/ BOTH1 / BOTH2	Sets the comparator judgment beeper setting	119
:CALCulate:LIMit:BEEPer?	OFF/ HL/ IN/ BOTH1 / BOTH2	Queries the comparator judgment beeper setting	119
:CALCulate:LIMit:RESistance:MODE	HL/ REF	Sets the resistance comparator execution mode setting	119
:CALCulate:LIMit:RESistance:MODE?	HL/ REF	Queries the resistance comparator execution mode setting	119
:CALCulate:LIMit:VOLTage:MODE	HL/ REF	Sets the voltage comparator execution mode setting	119
:CALCulate:LIMit:VOLTage:MODE?	HL/ REF	Queries the voltage comparator execution mode setting	119
:CALCulate:LIMit:RESistance:UPPer	<Upper threshold>	Sets the resistance comparator upper threshold setting	120
:CALCulate:LIMit:RESistance:UPPer?	<Upper threshold>	Queries the resistance comparator upper threshold setting	120
:CALCulate:LIMit:VOLTage:UPPer	<Upper threshold>	Sets the voltage comparator upper threshold setting	120
:CALCulate:LIMit:VOLTage:UPPer?	<Upper threshold>	Queries the voltage comparator upper threshold setting	120
:CALCulate:LIMit:RESistance:LOWer	<Lower threshold>	Sets the resistance comparator lower threshold setting	121
:CALCulate:LIMit:RESistance:LOWer?	<Lower threshold>	Queries the resistance comparator lower threshold setting	121
:CALCulate:LIMit:VOLTage:LOWer	<Lower threshold>	Sets the voltage comparator lower threshold setting	121
:CALCulate:LIMit:VOLTage:LOWer?	<Lower threshold>	Queries the voltage comparator lower threshold setting	121
:CALCulate:LIMit:RESistance:REFerence	<Reference value>	Sets the resistance comparator reference value	122
:CALCulate:LIMit:RESistance:REFerence?	<Reference value>	Queries the resistance comparator reference value	122
:CALCulate:LIMit:VOLTage:REFerence	<Reference value>	Sets the voltage comparator reference value	122
:CALCulate:LIMit:VOLTage:REFerence?	<Reference value>	Queries the voltage comparator reference value	122
:CALCulate:LIMit:RESistance:PERCent	<Tolerance (%)>	Sets the resistance comparator decision tolerance setting	123
:CALCulate:LIMit:RESistance:PERCent?	<Tolerance (%)>	Queries the resistance comparator decision tolerance setting	123
:CALCulate:LIMit:VOLTage:PERCent	<Tolerance (%)>	Sets the voltage comparator decision Tolerance setting	123
:CALCulate:LIMit:VOLTage:PERCent?	<Tolerance (%)>	Queries the voltage comparator decision tolerance setting	123
:CALCulate:LIMit:RESistance:RESult?	HI/ IN/ LO/ OFF/ ERR	Queries resistance comparator judgment results	124
:CALCulate:LIMit:VOLTage:RESult?	HI/ IN/ LO/ OFF/ ERR	Queries voltage comparator judgment results	124
Statistical Functions			
:CALCulate:STATistics:STATe	1/ 0/ ON/ OFF	Sets statistical calculation function execution	124
:CALCulate:STATistics:STATe?	ON/ OFF	Queries the statistical calculation function execution setting	124
:CALCulate:STATistics:CLEAr		Clears statistical calculation results	124
:CALCulate:STATistics:RESistance:NUMBer?	<Total data count>, <Valid data count>	Queries the resistance data count	125

Message ([ ] = optional)	Data Contents ( ) = response data	Description	Ref page
:CALCulate:STATistics:VOLTage:NUMBer?	<Total data count>, <Valid data count>	Queries the voltage data count	125
:CALCulate:STATistics:RESistance:MEAN?	<Mean>	Queries the resistance mean value	125
:CALCulate:STATistics:VOLTage:MEAN?	<Mean>	Queries the voltage mean value	125
:CALCulate:STATistics:RESistance:MAXimum?	<Maximum value>, <Data No. of Maximum value>	Queries the resistance maximum value	126
:CALCulate:STATistics:VOLTage:MAXimum?	<Maximum value>,<Data No. of Maximum value>	Queries the voltage maximum value	126
:CALCulate:STATistics:RESistance:MINimum?	<Minimum value>, <Data No. of Maximum value>	Queries the resistance minimum value	126
:CALCulate:STATistics:VOLTage:MINimum?	<Minimum value>, <Data No. of Maximum value>	Queries the voltage minimum value	126
:CALCulate:STATistics:RESistance:LIMit?	<Hi count>,<IN count>, <Lo count>, <Measurement fault count >	Queries comparator results of resistance measurement	127
:CALCulate:STATistics:VOLTage:LIMit?	<Hi count>,<IN count>, <Lo count>, <Measurement fault count >	Queries comparator results of voltage measurement	127
:CALCulate:STATistics:RESistance:DEViation?	<σn>, <σn-1>	Queries standard deviation of resistance measurement	127
:CALCulate:STATistics:VOLTage:DEViation?	<σn>, <σn-1>	Queries standard deviation of voltage measurement	127
:CALCulate:STATistics:RESistance:CP?	<Cp>, <CpK>	Queries process capability indices of resistance measurement	128
:CALCulate:STATistics:VOLTage:CP?	<Cp>, <CpK>	Queries process capability indices of voltage measurement	128
Memory Function			
:MEMory:STATe	1/ 0/ ON/ OFF	Sets the memory function state	128
:MEMory:STATe?	ON/ OFF	Queries the memory function state	128
:MEMory:CLEAr		Clears instrument memory	128
:MEMory:COUNt?	0 to 400	Queries the memory data count	129
:MEMory:DATA?	[STEP]	Queries the memory data	129
Self-Calibration			
:SYSTem:CALibration		Executes self-calibration	130
:SYSTem:CALibration:AUTO	1/ 0/ ON/ OFF	Sets automatic self-calibration	130
:SYSTem:CALibration:AUTO?	ON/ OFF	Queries the automatic self-calibration setting	130
Trigger Input Measured Value Ouputput			
:SYSTem:DATAout	1/ 0/ ON/ OFF	Sets measurement value output upon triggering	130
:SYSTem:DATAout?	ON/ OFF	Queries measurement value output upon triggering	130
Key Beeper			
:SYSTem:BEEPer:STATe	1/ 0/ ON/ OFF	Sets the key beeper	131
:SYSTem:BEEPer:STATe?	ON/ OFF	Queries the key beeper setting	131

Message ([ ] = optional)	Data Contents ( ) = response data	Description	Ref page
Line Frequency			
:SYSTem:LFRequency	50/ 60	Selects the AC line frequency	131
:SYSTem:LFRequency?	50/ 60	Queries the AC line frequency selection	131
Key-Lock			
:SYSTem:KLOCk	1/ 0/ ON/ OFF	Sets the key-lock	131
:SYSTem:KLOCk?	ON/ OFF	Queries the key-lock setting	131
EXT I/O Output			
:SYSTem:ELOCk	1/ 0/ ON/ OFF	Sets the external input terminal lock	132
:SYSTem:ELOCk?	ON/ OFF	Queries the external input terminal lock on/off setting	132
Local			
:SYSTem:LOCal		Sets local control	132
Saving and Loading Measurement Setting States			
:SYSTem:SAVE	<Table No.>	Saves the measurement setting state	132
:SYSTem:LOAD	<Table No.>	Loads a measurement setting state	132
:SYSTem:BACKup		Backups current measurement configuration	132
Header Present			
:SYSTem:HEADer	1/ 0/ ON/ OFF	Sets header present	133
:SYSTem:HEADer?	ON/ OFF	Queries the header present setting	133
ERR Output			
:SYSTem:ERRor	SYNChronous/ ASYNchronous	Sets error output timing	133
:SYSTem:ERRor?	SYNChronous/ ASYNchronous	Queries the error output timing setting	133
Terminator			
:SYSTem:TERMinator	0/ 1	Sets the terminator	133
:SYSTem:TERMinator?	0/ 1	Queries the terminator	133
System Reset			
:SYSTem:RESet		Executes a system reset, including saved measurement setting state data	134
EXT I/O			
:IO:OUT	0 to 1023	EXT I/O output	134
:IO:IN?	0 to 31	EXT I/O input	134
Trigger			
:INITiate:CONTinuous	1/ 0/ ON/ OFF	Sets continuous measurement	137
:INITiate:CONTinuous?	ON/ OFF	Queries the continuous measurement setting	137

Message ([ ] = optional)	Data Contents ( ) = response data	Description	Ref page
:INITiate[:IMMediate]		Trigger wait setting	137
Trigger Source Setting			
:TRIGger:SOURce	IMMediate/ EXTernal	Sets the trigger source	138
:TRIGger:SOURce?	IMMediate/ EXTernal	Queries the trigger source setting	138
:TRIGger:DELay:STATe	1/ 0/ ON/ OFF	Sets the trigger delay	138
:TRIGger:DELay:STATe?	ON/ OFF	Queries the trigger delay setting	138
:TRIGger:DELay	<Delay time>	Sets trigger delay time	139
:TRIGger:DELay?	0 to 9.999	Queries the trigger delay time	139
Reading Measured Values			
:FETCh?	<Resistance measured value>, <Voltage measured value> ΩV mode <Resistance measured value> Ω mode <Voltage measured value> V mode	Reads the most recent measurement	139
:READ?	<Resistance measured value>, <Voltage measured value> ΩV mode <Resistance measured value> Ω mode <Voltage measured value> V mode	Executes a measurement and read the measured values	140

7.6 Message Reference

< >: Indicates the contents (character or numeric parameters) of the data portion of a message.
Character parameters are returned as all capital letters.

Numeric Parameters:
- NRfNumber format may be any of NR1, NR2 and NR3
- NR1Integer data(e.g.: +12, -23, 34)
- NR2Fixed-point data(e.g.: +1.23, -23.45, 3.456)
- NR3Floating-point exponential representation data (e.g.: +1.0E-2, -2.3E+4)

Shows the command description.
Shows the message syntax.
Explains the command data or response message.

Describes the message.

Shows an example of an actual command application.
(Normally described with HEADER ON, (except the HEADER command itself).)

Read/Write the Standard Event Status Enable Register (SESER)

Syntax
Command *ESE <0 to 255 (NR1)>
Query *ESE?
Response <0 to 255 (NR1)>

Description
Command: The SESER mask is set to the numerical value 0 to 255.
The initial value (at power-on) is 0.
Query: The contents of the SESER, as set by the *ESE command, are returned as an NR1 value (0 to 255).

128	64	32	16	8	4	2	1
bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
PON	URQ	CME	EXE	DDE	QYE	RQC	OPC

Example
Command *ESE 36
(Sets bits 5 and 2 of SESER)

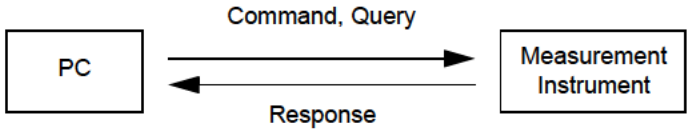

7.6.1 Standard Commands

Messages specific to the RS-232C or GP-IB interface are identified by their corresponding symbols.

System Data Command

Queries device ID.

Syntax Query `*IDN?`

Response <Manufacturer's name>,<Model name>,0,<Software version>

Description Query Queries the device manufacturer's name, model name and software version.

Example Query `*IDN?`

Response `HIOKI,3561,0,V1.00`
The Device ID is HIOKI 3561, 0, software version 1.00.

Note
- The response message has no header.
- The model name of the Model 3561-01 is "3561-01".

Internal Operation Command

Initialize Device

Syntax Command `*RST`

Description Command Resets instrument settings (other than saved data) to factory defaults. Operation returns to the initial display after initialization.

Note
- The communications state is not initialized.
- To initialize saved data as well, send the `:SYSTem:RESet` command.

Execute Self-Test and Query the Result

Syntax Query `*TST?`

Response <0 to 3>
0.....No Errors
1.....RAM Error
2.....EEPROM Error
3.....RAM and EEPROM Errors

Description Query Perform instrument self-test and return the result as numerical value 0 to 3.

Example Query `*TST?`

Response `1`
A RAM Error occurred.

Synchronization Commands

Set the OPC bit of SESR When Finished All Pending Operations

Syntax Command `*OPC`

Description Command Sets OPC bit 0 of the Standard Event Status Register (SESR) when all prior commands have finished processing.

Example Command `A;B;*OPC;C`
The OPC bit of the SESR is set after commands A and B have finished processing.

Respond "1" When Finished All Pending Operations

Syntax Query `*OPC?`

Response 1

Description Query Responds "1" when all prior commands have finished processing.

Wait for Pending Commands to Finish

Syntax Command `*WAI`

Description Command The instrument waits until all prior commands finish before executing any subsequent commands.

Note The `*WAI` command is supported because it is defined in IEEE 488.2-1987, but because all Model 3561(3561-01) device-specific commands are sequential types, this command has no actual affect.

Status and Event Control Commands

Clear the Status Byte and Related Queues (Except the Output Queue)

Syntax Command `*CLS`

Description Command Clears the event registers corresponding to each bit of the Status Byte Register. Also clears the Status Byte Register.

Note RS-232C The output queue is unaffected.

GP-IB The output queue, the various enable registers and MAV bit 4 of the
Status Byte Register are unaffected.

Set and Query the Standard Event Status Enable Register (SESER)

Syntax

Command `*ESE <0 to 255>`

Query `*ESE?`

Response <0 to 255 (NR1)>

Description

Command The SESER mask is set to the numerical value 0 to 255.
The initial value (at power-on) is 0.

Query The contents of the SESER, as set by the `*ESE` command, are returned as an NR1 value (0 to 255).

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
PON	URQ	CME	EXE	DDE	QYE	RQC	OPC

Example

Command `*ESE 36`
Sets bits 5 and 2 of SESER.

Query `*ESE?`

Response `36`
SESER havs been set to bit 5 and bit 2.

Query and Clear the Standard Event Status Register (SESR)

Syntax

Query `*ESR?`

Response <0 to 255 (NR1)>

Description

Query Returns the contents of the SESR as an NR1 value from 0 to 255, then clears register contents.
The response message has no header.

RS-232C

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
PON	unused	CME	EXE	DDE	QYE	unused	unused

GP-IB

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
PON	URQ	CME	EXE	DDE	QYE	RQC	OPC

Example

Query `*ESR?`

Response `32`
Bit 5 of the SESR was set to 1.

Set and Query the Service Request Enable Register (SRER)

Syntax

Command ∗**SRE** <0 to 255>

Query ∗**SRE?**

Response <0 to 255 (NR1)>

Description

Command The SRER mask is set to the numerical value 0 to 255.
Although NRf numerical values are accepted, values to the right of the decimal are rounded to the nearest integer.
Bit 6 and unused bits 2, 3 and 7 are ignored.
The data is initialized to zero at power-on.

Query The contents of the SRER, as set by the ∗**SRE** command, are returned as an NR1 value (0 to 255). Bit 6 and unused bits 2, 3 and 7 always return as zero.

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
unused	0	ESB	MAV	unused	unused	ESE1	ESE0

Example

Command ∗**SRE 33**
Set SRER bits 0 and 5 to 1.

Query ∗**SRE?**

Response **33**
SRER bits 0 and 5 have been set to 1.

Query the Status Byte and MSS Bit

Syntax

Query ∗**STB?**

Response <0 to 255 (NR1)>

Description

Query The contents of the STB are returned as an NR1 value (0 to 255). The response message has no header.

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
unused	MSS	ESB	MAV	unused	unused	ESE1	ESE0

Example

Query ∗**STB?**

Response **16**
STB bit 4 has been set to 1.

Request a Sample

Syntax

Command ∗**TRG**

Description

Command Performs one measurement when external triggering is enabled.
When Statistical Calculation is ON, imports calculation data.

7.6.2 Device-Specific Commands

Set and Query Device-Specific Event Status Enable Registers ESER0

Syntax

Command `:ESE0` <0 to 255>

Query `:ESE0?`

Response <0 to 255 (NR1)>

Description

Command Sets the mask pattern in Event Status Enable Register 0 (ESER0) for the Event Status Register.

Query Queries the mask pattern in Event Status Enable Register 0 (ESER0) for the Event Status Register.

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
unused	unused	ERR	unused	unused	unused	INDEX	EOC

Note Data initializes to zero at power-on.

Set and Query Device-Specific Event Status Enable Registers ESER1

Syntax

Command `:ESE1` <0 to 255>

Query `:ESE1?`

Response <0 to 255 (NR1)>

Description

Command Sets the mask pattern in Event Status Enable Register 1 (ESER1) for the Event Status Register.

128 bit 7	64 bit 6	32 bit 5	16 bit 4	8 bit 3	4 bit 2	2 bit 1	1 bit 0
unused	AND	V-Hi	V-IN	V-Lo	R-Hi	R-IN	R-Lo

Note Data initializes to zero at power-on.

Read Device-Specific Event Status Registers ESR0 and ESR1

Syntax

Query `:ESR0?`
`:ESR1?`

Response <0 to 255 (NR1)>

Note Executing `:ESR0?` clears the contents of ESR0.
Executing `:ESR1?` clears the contents of ESR1.

Select and Query the Measurement Mode Setting

Syntax

Command **:FUNCtion** <RV/ RESistance/ VOLTage>

Query **:FUNCtion?**

Response <RV/ RESISTANCE/ VOLTAGE>
RV.....ΩV mode
(Resistance and voltage measurement)
RESISTANCE ....Ω mode (Resistance measurement)
VOLTAGE .....V mode (Voltage measurement)

Example

Command **:FUNC RV**
Selects the ΩV mode.

Query **:FUNC?**

Response **RV**
ΩV mode has been selected.

Set and Query the Resistance Measurement Range

Syntax

Command **:RESistance:RANGe** < 0 to 3.1>

Query **:RESistance:RANGe?**

Response <300.00E-3/ 3.0000E+0 (NR3)>

Example

Command **:RES:RANG 120E-3**
Selects the most suitable resistance measurement range for measuring 120 mΩ.

Query **:RES:RANG?**
Response **300.00E-3**
The current resistance measurement range is 300 mΩ.

Note Changing the resistance measurement range clears stored measurement data (memory function).

Set and Query the Voltage Measurement Range

Syntax

Command **:VOLTage:RANGe** <-20 to 20>

Query **:VOLTage:RANGe?**

Response <20.0000E+0 (NR3)>

Example

Command **:VOLT:RANG 15**
Selects the voltage measurement range for measuring 15 V.

Query **:VOLT:RANG?**
Response **20.0000E+0**
The voltage measurement range is fixed at 20 V (single range).

Set and Query the Auto-Ranging Setting

Syntax
Command `:AUTorange` <1, 0, ON or OFF>
Query `:AUTorange?`
Response <ON or OFF>

Example
Command `:AUT ON`

Note
- Attempting to enable auto-ranging when the Comparator or Memory function is enabled results in a execution error.
- Because there is only one voltage range (20 V), auto-ranging does not apply to voltage measurement.

Cancel Zero-Adjustment

Syntax
Command `:ADJust:CLEAr`

Description
Command Clears zero adjustment.

Execute Zero Adjustment and Query the Result

Syntax
Query `:ADJust?`
Response <0/ 1 (NR1)>
0.....Zero adjustment succeeded
1.....Zero adjustment failed
The acceptable range of zero adjustment for both resistance and voltage is ± 1,000 dgt.

Description
Query Queries whether zero adjustment has succeeded or failed.

Example
Query `:ADJ?`
Response 0
Zero adjustment executed successfully.

Select and Query the Sampling Rate setting

Syntax
Command `:SAMPle:RATE` <EXFast/ FAST/ MEDium/ SLOW>
Query `:SAMPle:RATE?`
Response <EXFAST/ FAST/ MEDIUM/ SLOW>

Example
Command `:SAMP:RATE MED`
Query `:SAMP:RATE?`
Response `MEDIUM`

Set and Query the Averaging Function Setting

Syntax
Command `:CALCulate:AVERage:STATe` <1, 0, ON or OFF>
Query `:CALCulate:AVERage:STATe?`
Response <ON or OFF>

Example
Command `:CALC:AVER:STAT OFF`
Query `:CALC:AVER:STAT?`
Response `OFF`

Set and Query the No. of samples to average

Syntax
Command `:CALCulate:AVERage` <2 to 16>
Query `:CALCulate:AVERage?`
Response <2 to 16 (NR1)>

Example
Command `:CALC:AVER 10`
Query `:CALC:AVER?`
Response `10`

Set and Query the Comparator

Syntax
Command `:CALCulate:LIMit:STATe` <1, 0, ON or OFF>
Query `:CALCulate:LIMit:STATe?`
Response <ON or OFF>

Example
Command `:CALC:LIM:STAT ON`
Query `:CALC:LIM:STAT?`
Response `ON`

Note
- When the Comparator function is enabled, auto-ranging is disabled.
- Switching the Comparator function on/off or changing its settings clears stored measurement data (memory function).

Set and Query Comparator Judgments

Syntax

Command `:CALCulate:LIMit:BEEPer` <OFF/HL/IN/BOTH1/BOTH2>

Query `:CALCulate:LIMit:BEEPer?`

Response <OFF/ HL/ IN/ BOTH1/ BOTH2>

OFF.....No beeps sound.
HL .....The beeper sounds upon Hi and Lo judgments.
IN .....The beeper sounds upon IN judgments.
BOTH1.....The beeper sounds continuously upon IN judgments, and repeatedly upon Hi and Lo judgments.
BOTH2.....The beeper sounds once (briefly) upon IN judgments, and repeatedly upon Hi and Lo judgments.

Example

Command `:CALC:LIM:BEEP IN`

Query `:CALC:LIM:BEEP?`

Response `IN`

Set and Query the Comparator Execution Mode Setting

(Resistance Measurement)

Syntax

Command `:CALCulate:LIMit:RESistance:MODE` <HL/ REF>

Query `:CALCulate:LIMit:RESistance:MODE?`

Response <HL/ REF>

HL .....Decision by preset upper and lower thresholds.
REL.....Decision by a reference value and tolerance.

Example

Command `:CALC:LIM:RES:MODE REF`

Query `:CALC:LIM:RES:MODE?`

Response `REF`

(Voltage Measurement)

Syntax

Command `:CALCulate:LIMit:VOLTage:MODE` <HL/ REF>

Query `:CALCulate:LIMit:VOLTage:MODE?`

Response <HL/ REF>

HL .....Decision by preset upper and lower thresholds.
REL.....Decision by a reference value and tolerance.

Set and Query the Comparator Upper Threshold Setting

(Resistance Measurement)

Syntax

Command `:CALCulate:LIMit:RESistance:UPPer` <Upper threshold>

Query `:CALCulate:LIMit:RESistance:UPPer?`

Response <Upper threshold>
<Upper threshold> = 0 to 99999 (NR1)

Example

Command `:CALC:LIM:RES:UPP 28593`
Sets the upper threshold to 285.93 mΩ (with the 300 mΩ range selected)
(If the 3 Ω range is selected, the threshold is set to 2.8593 Ω)

Query `:CALC:LIM:RES:UPP?`

Response `28593`

Note The value is sent as a whole integer (count). To set 120.53 mΩ with the 300 mΩ range, send the following:
`:CALC:LIM:RES:UPP 12053`

(Voltage Measurement)

Syntax

Command `:CALCulate:LIMit:VOLTage:UPPer` <Upper threshold>

Query `:CALCulate:LIMit:VOLTage:UPPer?`

Response <Upper threshold>
<Upper threshold> = 0 to 999999 (NR1)

Example

Command `:CALC:LIM:VOLT:UPP 39500`
Sets the upper threshold to 3.9500 V.

Query `:CALC:LIM:VOLT:UPP?`

Response `39500`

Note The value is sent as a whole integer (count).
To set 15.2005 V, send the following command:
`:CALC:LIM:VOLT:UPP 152005`

Set and Query the Comparator Lower Threshold Setting

(Resistance Measurement)

Syntax

Command
```
:CALCulate:LIMit:RESistance:LOWer
```
<Lower threshold>

Query
```
:CALCulate:LIMit:RESistance:LOWer?
```

Response
<Lower threshold>
<Lower threshold> = 0 to 99999 (NR1)

Example

Command
```
:CALC:LIM:RES:LOW 28406
```
Sets the lower threshold to 284.06 mΩ (with the 300 mΩ range selected)
(If the 3 Ω range is selected, the threshold is set to 2.8406 Ω)

Query
```
:CALC:LIM:RES:LOW?
```

Response
```
28406
```

Note

The value is sent as a whole integer (count). To set 120.53 mΩ with the 300 mΩ range, send the following:
```
:CALC:LIM:RES:LOW 12053
```

(Voltage Measurement)

Syntax

Command
```
:CALCulate:LIMit:VOLTage:LOWer
```
<Lower threshold>

Query
```
:CALCulate:LIMit:VOLTage:LOWer?
```

Response
<Lower threshold>
<Lower threshold> = 0 to 999999 (NR1)

Example

Command
```
:CALC:LIM:VOLT:LOW 37500
```
Sets the lower threshold to 3.7500 V.

Query
```
:CALC:LIM:VOLT:LOW?
```

Response
```
37500
```

Note

The value is sent as a whole integer (count).
To set 15.2005 V, send the following command:
```
:CALC:LIM:VOLT:LOW 152005
```

Set and Query the Comparator Reference Value

(Resistance Measurement)

Syntax

Command: `:CALCulate:LIMit:RESistance:REFerence <Reference value>`

Query: `:CALCulate:LIMit:RESistance:REFerence?`

Response: <Reference value>
<Reference value> = 0 to 99999 (NR1)

Example

Command: `:CALC:LIM:RES:REF 5076`
Sets the reference value to 50.76 mΩ (with the 300 mΩ range selected)
(If the 3 Ω range is selected, the threshold is set to 0.5076 Ω)

Query: `:CALC:LIM:RES:REF?`

Response: `5076`

Note

The value is sent as a whole integer (count). To set 120.53 mΩ with the 300 mΩ range, send the following:
`:CALC:LIM:RES:REF 12053`

(Voltage Measurement)

Syntax

Command: `:CALCulate:LIMit:VOLTage:REFerence <Reference value>`

Query: `:CALCulate:LIMit:VOLTage:REFerence?`

Response: <Reference value>
<Reference value> = 0 to 999999 (NR1)

Example

Command: `:CALC:LIM:VOLT:REF 38500`
Sets the reference value to 3.8500 V.

Query: `:CALC:LIM:VOLT:REF?`

Response: `38500`

Note

The value is sent as a whole integer (count).
To set 15.2005 V, send the following command:
`:CALC:LIM:VOLT:REF 152005`

Set and Query the Comparator Decision Tolerance Setting (Comparator Function)

(Resistance Measurement)

Syntax

Command
```
:CALCulate:LIMit:RESistance:PERCent
```
<Tolerance (%)>

Query
```
:CALCulate:LIMit:RESistance:PERCent?
```

Response
<Tolerance (%)>
<Tolerance (%)> = 0 to 99.999 (NR2)

Example

Command
```
:CALC:LIM:RES:PERC 0.3
```

Query
```
:CALC:LIM:RES:PERC?
```

Response
```
0.300
```

(Voltage Measurement)

Syntax

Command
```
:CALCulate:LIMit:VOLTage:PERCent
```
<Tolerance (%)>

Query
```
:CALCulate:LIMit:VOLTage:PERCent?
```

Response
<Tolerance (%)>
<Tolerance (%)> = 0 to 99.999 (NR2)

Example

Command
```
:CALC:LIM:VOLT:PERC 1.538
```

Query
```
:CALC:LIM:VOLT:PERC?
```

Response
```
1.538
```

Query Comparator Judgment Results

(Resistance Measurement)

Syntax Query `:CALCulate:LIMit:RESistance:RESult?`

Response <HI/ IN/ LO/ OFF/ ERR>

Example Query `:CALC:LIM:RES:RES?`

Response `HI`

(Voltage Measurement)

Syntax Query `:CALCulate:LIMit:VOLTage:RESult?`

Response <HI/ IN/ LO/ OFF/ ERR>

Execute Statistical Functions

Syntax Command `:CALCulate:STATistics:STATe` <1, 0, ON or OFF>

Query `:CALCulate:STATistics:STATe?`

Response <ON or OFF>

Example Command `:CALC:STAT:STAT ON`

Query `:CALC:STAT:STAT?`

Response `ON`

NOTE

About the Statistical Calculation function

Data samples can be acquired by the following three methods:

- Press the **TRIG** key
- Apply an EXT I/O TRIG signal
- Send the `*TRG` command

The `:CALCulates:STATistics:STATe` command does not clear calculation results.

When the valid data count is zero, σ_{n-1} returns 0.

Clearing calculation results does not disable the Statistical Calculation function.

The upper limit of Cp and CpK is 99.99. Cp and CpK values greater than 99.99 are returned as 99.99.

The lower limit of Cp and CpK is 0. Cp and CpK values less than 0 are returned as 0.00.

Clear Statistical Calculation Results

Syntax Command `:CALCulate:STATistics:CLEAr`

Query the Data Count

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:NUMBer?`

Response <Total data count (NR1)>,<Valid data count (NR1)>
<Total data count (NR1)> = 0 to 30000 (NR1)
<Valid data count (NR1)> = 0 to 30000 (NR1)

Example Query `:CALC:STAT:RES:NUMB?`

Response `22,20`

Note Measurement faults and out-of-range "OF" measurements are ignored for statistical calculations.

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:NUMBer?`

Response <Total data count (NR1)>,<Valid data count (NR1)>

Example Query `:CALC:STAT:VOLT:NUMB?`

Response `22,20`

Note Measurement faults and out-of-range "OF" measurements are ignored for statistical calculations.

Query the Mean value

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:MEAN?`

Response <Mean (NR3)>

Example Query `:CALC:STAT:RES:MEAN?`

Response `295.76E-3`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:MEAN?`

Response <Mean (NR3)>

Example Query `:CALC:STAT:VOLT:MEAN?`

Response `1.3923E+0`

Query the Maximum value

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:MAXimum?`

Response <Maximum value (NR3)>,<Data No. of Maximum value (NR1)>

Example Query `:CALC:STAT:RES:MAX?`

Response `297.28E-3,15`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:MAXimum?`

Response <Maximum value (NR3)>,<Data No. of Maximum value (NR1)>

Example Query `:CALC:STAT:VOLT:MAX?`

Response `1.3924E+0,1`

Query the Minimum value

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:MINimum?`

Response <Minimum value (NR3)>,<Data No. of Minimum value (NR1)>

Example Query `:CALC:STAT:RES:MIN?`

Response `294.88E-3,8`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:MINimum?`

Response <Minimum value (NR3)>,<Data No. of Minimum value (NR1)>

Example Query `:CALC:STAT:VOLT:MIN?`

Response `1.3923E+0,2`

Query Comparator Judgment Results (Statistical Calculation Function)

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:LIMit?`

Response <Hi (NR1) count>,<IN (NR1) count>,<Lo (NR1) count>,
<Measurement fault count (NR1)>

Example Query `:CALC:STAT:RES:LIM?`

Response `6,160,13,2`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:LIMit?`

Response <Hi (NR1) count>,<IN (NR1) count>,
<Lo (NR1) count>,<Measurement fault count (NR1)>

Example Query `:CALC:STAT:VOLT:LIM?`

Response `1,19,0,2`

Query Standard Deviation

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:DEViation?`

Response <σ_n (NR3)>,<σ_{n-1} (NR3)>

Example Query `:CALC:STAT:RES:DEV?`

Response `0.82E-3,0.84E-3`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:DEViation?`

Response <σ_n (NR3)>,<σ_{n-1} (NR3)>

Example Query `:CALC:STAT:VOLT:DEV?`

Response `0.0000E+0,0.0000E+0`

Query the Process Capability Indices

(Resistance Measurement)

Syntax Query `:CALCulate:STATistics:RESistance:CP?`

Response <Cp (NR2)>,<CpK (NR2)>

Example Query `:CALC:STAT:RES:CP?`

Response `0.04, 0.04`

(Voltage Measurement)

Syntax Query `:CALCulate:STATistics:VOLTage:CP?`

Response <Cp (NR2)>,<CpK (NR2)>

Example Query `:CALC:STAT:VOLT:CP?`

Response `0.91, 0.00`

Set and Query the Memory Function State

Syntax Command `:MEMory:STATe` <1/0/ON/OFF>

Query `:MEMory:STATe?`

Response <ON/OFF>

Example Command `:MEM:STAT ON`

Query `:MEM:STAT?`

Response `ON`

Clear Instrument Memory

Syntax Command `:MEMory:CLEAr`

Query the Memory Data Count

Syntax

Query `:MEMory:COUNt?`

Response <Memory data count>
<Memory data count> = 0 to 400 (NR1)

Example

Query `:MEM:COUN?`

Response `5`

Query (Download) Memory Data

Syntax

Query `:MEMory:DATA? [STEP]`

Response <Memory data No. (NR1)>,<Measured resistance (NR3)>,<Measured voltage (NR3)>
Memory data values are returned as data objects.
If [STEP] is omitted, all memory data objects are returned continuously.

Example

Query `:MEM:DATA?`

Example

Response
```
  1,  290.60E-3,  1.3924E+0
  2,  290.54E-3,  1.3924E+0
  3,  290.50E-3,  1.3923E+0
  4,  290.43E-3,  1.3923E+0
  5,  290.34E-3,  1.3924E+0
END
```

Query `:MEM:DATA? STEP`

Response
```
  1,  290.60E-3,  1.3924E+0
N (Sent from PC)
  2,  290.54E-3,  1.3924E+0
N (Sent from PC)
  3,  290.50E-3,  1.3923E+0
N (Sent from PC)
  4,  290.43E-3,  1.3923E+0
N (Sent from PC)
  5,  290.34E-3,  1.3924E+0
N (Sent from PC)
END
```

Note

- Stored memory data objects are returned continuously, or one data object at a time. The “END” character is returned as the last data object. When the “STEP” parameter is specified, one data object is returned at a time. Sending “N” to the instrument after receiving the data causes the next data object to be returned. The memory index is an unsigned three-digit integer. Refer to “Measurement Value Formats” for format details of returned measurement values.
- A terminator is appended to the end of each returned memory data object. When sending “N” from the PC or other device, a terminator is required.
  ❖See Section Message Terminators (Page 94).
- Measured values are stored in memory when pressing the **TRIG** key, applying a signal to the $\overline{\text{TRIG}}$ EXT I/O connector or sending the `*TRG` command (while the Memory function is enabled). Up to 400 data objects can be stored. When the memory is full, additional measurement data is not stored.
- When the Memory function is enabled, auto-ranging is disabled.

Execute Self-Calibration

Syntax Command **:SYSTem:CALibration**

Self-Calibration State and Setting

Command **:SYSTem:CALibration:AUTO** <1, 0, ON or OFF>

Query **:SYSTem:CALibration:AUTO?**

Response <ON or OFF>
ON... AUTO Self-Calibration selected
(executes approximately every 30 minutes)
OFF MANUAL Self-Calibration selected

Example Command **:SYST:CAL:AUTO ON**

Query **:SYST:CAL:AUTO?**
Response **ON**

Note Even when AUTO is selected, Self-Calibration can be manually performed at any time by sending the **:SYSTem:CALibration** command.

Set and Query Measurement Value Output Upon Triggering

Command **:SYSTem:DATAout** <1, 0, ON or OFF>

Query **:SYSTem:DATAout?**

Response <ON or OFF>
ON... Measured values are output automatically when a trigger occurs.
OFF Measured values are not output.

Example Command **:SYST:DATA OFF**

Query **:SYST:DATA?**

Response **OFF**

Note
- This function is convenient when you want to obtain measured values by applying EXT I/O trigger input. When this function is enabled and a footswitch is connected to the $\overline{\text{TRIG}}$ terminal of the EXT I/O connector, a measured value is sent to the PC automatically each time the footswitch is pressed, so there is no need to send a command from the PC to obtain measurement values.
- Refer to "Measurement Value Formats" for format details of returned measurement values.
- This function is not available when the GP-IB interface is selected.
❖See Section 4.10 Measurement Value Output Function (Page 64).

Set and Query the Key Beeper Setting

Syntax
Command `:SYSTem:BEEPer:STATe` <1, 0, ON or OFF>
Query `:SYSTem:BEEPer:STATe?`
Response <ON or OFF>

Example
Command `:SYST:BEEP:STAT ON`
Query `:SYST:BEEP:STAT?`
Response `ON`

Note Only key-press beeps are set on or off. Comparator judgment beeps are unaffected.

Select and Query the Line Frequency Setting

Syntax
Command `:SYSTem:LFRequency` <50/ 60>
Query `:SYSTem:LFRequency?`
Response <50/ 60>

Example
Command `:SYST:LFR 60`
Query `:SYST:LFR?`
Response `60`

Set and Query the Key-Lock State

Syntax
Command `:SYSTem:KLOCk` <1, 0, ON or OFF>
Query `:SYSTem:KLOCk?`
Response <ON or OFF>

Example
Command `:SYST:KLOC ON`
Query `:SYST:KLOC?`
Response `ON`

Set and Query EXT I/O Lock

Syntax

Command `:SYSTem:ELOCk` <1, 0, ON or OFF>

Query `:SYSTem:ELOCk?`

Response <ON or OFF>
ON..... EXT I/O control is disabled (preventing inadvertent operations from electrical noise).
OFF..... EXT I/O control is enabled.

Example

Command `:SYST:ELOC ON`

Query `:SYST:ELOC?`

Response `ON`

Note This function affects only command input.

Set Local Control

Syntax

Command `:SYSTem:LOCal`

Note Switches from remote control (REMOTE indicator lit) to local control (by panel keys).

Save and Load Measurement Values

Syntax

Command `:SYSTem:SAVE` <1 to 126>
`:SYSTem:LOAD` <1 to 126>

Note

- Attempting to load a panel number that has not been saved results in an execution error.
- Up to 126 measurement configurations can be saved and loaded. Refer to “Panel Save and Load Functions” for details.

Backup Current Measurement Configuration

Syntax

Command `:SYSTem:BACKup`

Description

Command The current measurement configuration (settings) is backed up so that when power is turned on the next time, the same configuration is restored.

Note Saved panel and backup settings are stored in the instrument’s EEPROM. Be aware that the number of times that the EEPROM can be rewritten is limited (to about a million times).

Set and Query the Header Present Setting

Syntax
Command `:SYSTem:HEADer` <1, 0, ON or OFF>
Query `:SYSTem:HEADer?`
Response <ON or OFF>

Description
Command Specifies whether a header is sent with response messages.

Example
Command `:SYST:HEAD ON`
Query `:SYST:HEAD?`
Response `:SYSTEM:HEADER ON`
Command `:SYST:HEAD OFF`
Query `:SYST:HEAD?`
Response `:OFF`

Set and Query Error Output Timing

Syntax
Command `:SYSTem:ERRor` <SYNChronous/ ASYNchronous>
Query `:SYSTem:ERRor?`
Response <SYNCHRONOUS/ ASYNCHRONOUS>
SYNCHRONOUS ..... Synchronize with EOC output
ASYNCHRONOUS..... Asynchronous with EOC output

Example
Command `:SYST:ERR ASYN`
Query `:SYST:ERR?`
Response `ASYNCHRONOUS`

Set and Query the terminator

GP-IB

Syntax
Command `:SYSTem:TERMinator` <0/ 1>
Query `:SYSTem:TERMinator?`
Response <0/ 1>
0.....LF+EOI
1.....CR ,LF+EOI

Example
Command `:SYST:TERM 1`
Query `:SYST:TERM?`
Response 0

Note
The RS-232C delimiter is fixed as CR + LF.
❖See Section Message Terminators (Page 94).

System Reset

Syntax Command `:SYSTem:RESet`

Description Command All settings including saved panel settings are returned to factory defaults. Refer to “Reset Function” for details.

Example Command `:SYST:RES`

Note
- If you want to preserve saved data, use the `*RST` command instead.
- The communications settings are not re-initialized.

EXT I/O Output

Syntax Command `:IO:OUT` <0 to 1023>

Description Command Any 10-bit data can be output from the EXT I/O connectors.
❖See Section 5.2.3 Output Signals (Page 72).

	bit9	bit8	bit7	bit6	bit5	bit4	bit3	bit2	bit1	bit0
	OUT9	OUT8	OUT7	OUT6	OUT5	OUT4	OUT3	OUT2	OUT1	OUT0
Pin No.	36	18	35	17	34	16	33	15	32	14

EXT I/O Input

Syntax Query `:IO:IN?`

Response 0 to 31(NR1)

Description Query Signals at the EXT I/O ($\overline{IN0}$ to $\overline{IN4}$) input terminals are read at the leading edge.
Each bit (edge data) is cleared upon reading by this query.
A bit is set when the leading edge (short between each signal terminal and the GND terminal) is detected, and is cleared when read by this query command.
❖See Section 5.2.2 Input Signals (Page 71).

	bit4	bit3	bit2	bit1	bit0
	$\overline{IN4}$ ($\overline{MANU}$)	$\overline{IN3}$ ($\overline{PRINT}$)	$\overline{IN2}$ ($\overline{0ADJ}$)	$\overline{IN1}$ ($\overline{CAL}$)	$\overline{IN0}$ ($\overline{TRIG}$)
Pin No.	24	6	23	5	22

Note The **TRIG** key and `*TRG` command are detected in the same way as the TRIG terminal signal.

Triggering System Description

Triggering operates as follows depending on the continuous measurement setting (:INITIATE:CONTINUOUS) and the trigger source setting (:TRIGGER:SOURCE).
❖See Section 7.7 Basic Data Importing Methods (Page 146).

		Continuous Measurement (:INITIATE:CONTINUOUS)	
		ON	OFF*1
Trigger Source (:TRIGGER:SOURCE)	IMMEDIATE (EXT.TRIG not lit)	Free-Run state. Measurement continues automatically. ❖See next page (1)	Trigger by :INITIATE (or :READ?) command. ❖See next page (2)
	EXTERNAL (EXT.TRIG lit)	Trigger by TRIG terminal, TRIG key or *TRG command. After measurement, enters the trigger wait state. ❖See next page (3)	Issue :INITIATE (or :READ?) command to wait for trigger. Trigger by $\overline{\text{TRIG}}$ terminal, TRIG key or *TRG command. ❖See next page (4)*2

*1: :INITIATE:CONTINUOUS OFF
Can only be set by Remote command.
If this has been set to OFF when operation is returned to the Local state or power is turned off, the following state occurs when power is turned back on.
:INITIATE:CONTINUOUS ON
❖See Section 7.4.6 Local Function (Page 103).

*2: The *TRG command cannot be used for triggering while awaiting a trigger after issuing a :READ? command. In this case, use the $\overline{\text{TRIG}}$ terminal or TRIG key for triggering.

Measurement Flow

1 `:INITIATE:CONTINUOUS ON`
`:TRIGGER:SOURCE IMMEDIATE`

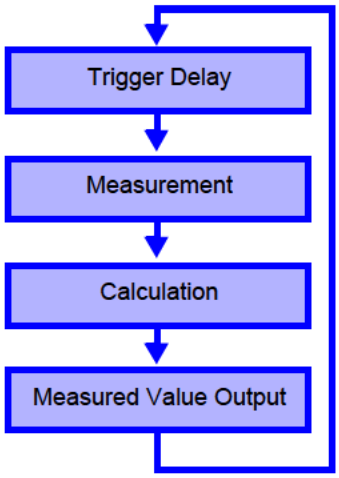

2 `:INITIATE:CONTINUOUS OFF`
`:TRIGGER:SOURCE IMMEDIATE`

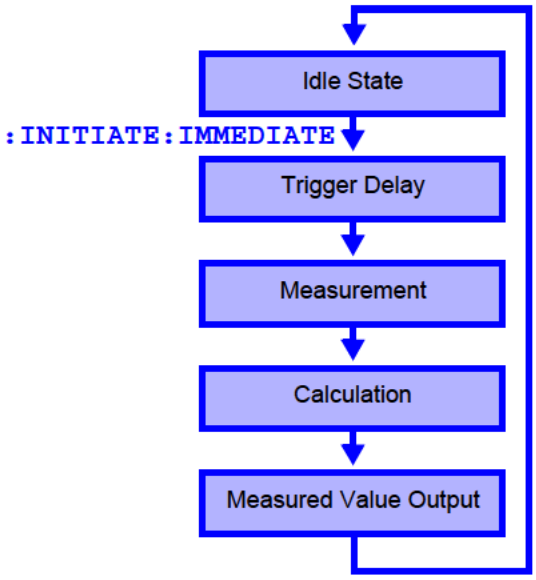

3 `:INITIATE:CONTINUOUS ON`
`:TRIGGER:SOURCE EXTERNAL`

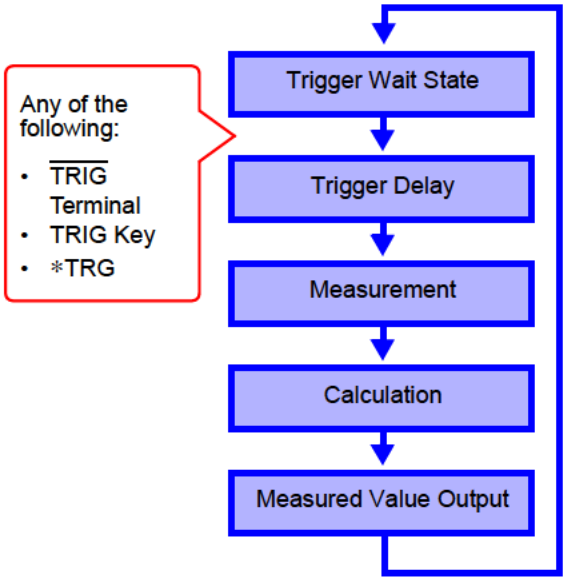

4 `:INITIATE:CONTINUOUS`
`OFF`
`:TRIGGER:SOURCE`

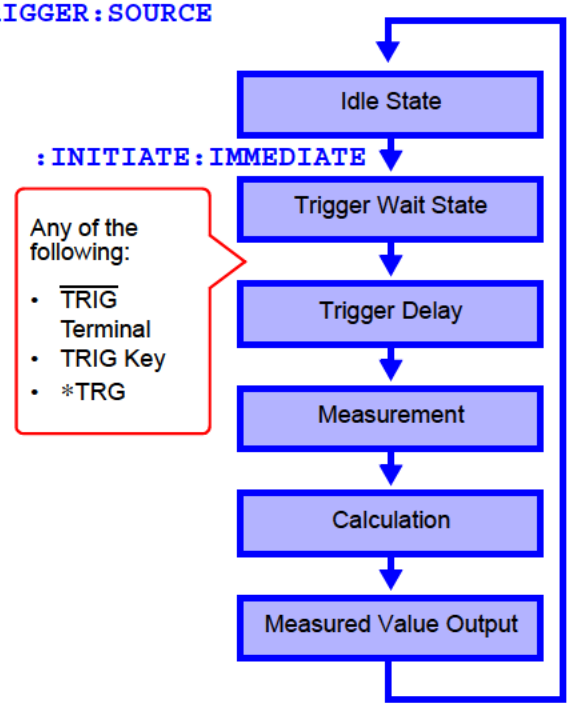

Continuous Measurement Setting

Syntax

Command `:INITiate:CONTinuous` <1, 0, ON or OFF>

Query `:INITiate:CONTinuous?`

Response <ON or OFF>
ON ..... Continuous Measurement Enabled
OFF ..... Continuous Measurement Disabled

Description

Command Sets continuous measurement.

Query Queries the continuous measurement setting.

Example

Command `:INIT:CONT OFF`
Disables continuous measurement.

Query `:INIT:CONT?`
Response `ON`
Enables continuous measurement.

Note

- Continuous Measurement Enabled:
  After measurement, enters the Trigger Wait State. When the trigger source setting is IMMediate, the next trigger occurs immediately (the Free-Run State).
- Continuous Measurement Disabled:
  After measurement, enters the Idle State instead of the Trigger Wait State.
- Triggering is ignored in the Idle State. Executing :INITiate[:IMMediate] enables the Trigger Wait State.
- Continuous measurement is enabled upon exit from the Remote State.

Trigger Wait Setting

Syntax

Command `:INITiate[:IMMediate]`

Description

Command Switches triggering from the Idle State to the Trigger Wait State.

Example

Command Disable continuous measurement, and read one value for each trigger event

Send
`:TRIG:SOUR IMM`... Trigger immediately when entering Trigger Wait State
`:INIT:CONT OFF`... Disables continuous measurement
`:INIT`..... Enable Trigger Wait Trigger immediately upon :TRIG:SOUR IMM
`:FETC?`..... Fetch measured value

Response `2.1641E+0` ..... Measured value is 2.1641 Ω

Error

- An execution error occurs when continuous measurement is enabled (`:INITIATE:CONTINUOUS ON`).

Note

- When the trigger source is IMMediate, triggering occurs immediately before entering the Idle State.
- When the trigger source is EXTernal, the Trigger Wait State is enabled to wait for an external trigger, and when a trigger occurs, one measurement is taken before entering the Idle State.

Set and Query the Trigger Source

Syntax

Command **:TRIGger:SOURce** <IMMediate/ EXTernal>

Query **:TRIGger:SOURce?**

Response <IMMEDIATE/ EXTERNAL>
IMMEDIATE .. Internal triggering
EXTERNAL ... External trigger source. Triggering by **TRIG** key, TRIG terminal or ***TRG** command.

Description

Command Selects the trigger source.

Query Queries the trigger source selection.

Example

Command **:TRIG:SOUR IMM**
Sets the trigger source to internal triggering.

Query **:TRIG:SOUR?**
Response **IMMEDIATE**
The trigger source is set to internal triggering.

Enable/Disable and Query Trigger Delay

Syntax

Command **:TRIGger:DELay:STATe** <1, 0, ON or OFF>

Query **:TRIGger:DELay:STATe?**

Response <ON or OFF>
ON..... Trigger delay enabled
OFF..... Trigger delay disabled

Example

Command **:TRIG:DEL:STAT ON**
Enables trigger delay.

Query **:TRIG:DEL:STAT?**
Response **ON**
Trigger delay is enabled (ON).

Set and Query Trigger Delay Interval

Syntax

Command: `:TRIGger:DELay` <0 to 9.999>

Query: `:TRIGger:DELay?`

Response: <0 to 9.999 (NR2)>

Description

Command: Sets the trigger delay interval.

Query: Queries the trigger delay interval setting.

Example

Command: `:TRIG:DEL 0.058`
Sets the trigger delay to 0.058 seconds.

Query: `:TRIG:DEL?`
Response: `0.058`
The trigger delay is set to 0.058 seconds.

Read the Latest Measurement

Syntax

Query: `:FETCh?`

Response:

<Measured resistance (NR3)>, <Measured voltage (NR3)>	(ΩV mode)
<Measured resistance (NR3)>	(Ω mode)
<Measured voltage (NR3)>	(V mode)

Description

Query: Reads the most recent measurement. No trigger occurs.

Example

Query: `:FETC?`
Response: `288.02E-3,1.3921E+0` (ΩV mode)
The last measured resistance is 288.02 mΩ, and the last measured voltage is 1.3921 V.
❖ See Section 7.6.3 Measurement Value Formats (Page 141).

Execute a Measurement and Read the Measured Values

Syntax

Query `:READ?`

Response <Measured resistance (NR3)>, <Measured voltage (NR3)> (ΩV mode)
<Measured resistance (NR3)> (Ω mode)
<Measured voltage (NR3)> (V mode)

Description

Query

Switches from the Idle State to the Trigger Wait State, then reads the next measured value. With auto-ranging enabled, the most suitable range is selected before measurement.

Trigger Source	Operation
IMMediate	Triggers and reads measured value.
EXTernal	After triggering by the $\overline{\text{TRIG}}$ terminal (EXT I/O) or **TRIG** key, reads the measured value.

Example

Query `:READ?`

Response `289.68E-3, 1.3921E+0` (ΩV mode)
Measured resistance is 289.68 mΩ, and voltage is 1.3921 V.

Error

This command causes an execution error if issued during the Continuous Measurement state (after `:INITIATE:CONTINUOUS ON`).

Note

- The next command does not execute until measurement is finished.
- When the trigger source is external, the `*TRG` command does not trigger measurement.

❖ See Section 7.6.3 Measurement Value Formats (Page 141).

7.6.3 Measurement Value Formats

For the commands that acquire measurement values (`:FETCH?` and `:READ?`), the response formats are as follows.

Measured Resistance

Measurement range	Measured Value	±OF	Measurement Fault
300 mΩ	±□□□□.□□E-3	±1000.00E+6	+1000.00E+7
3 Ω	±□□.□□□□E+0	±10.0000E+8	+10.0000E+9

Measured Voltage

Measurement range	Measured Value	±OF	Measurement Fault
20 V	±□□.□□□□E+0	±10.0000E+8	+10.0000E+9

Relative Value Indication
(same as voltage and resistance)

Measurement range	Measured Value	±OF	Measurement Fault
All ranges	±□□□.□□□E+0	±100.000E+7	+100.000E+8

For positive measurements, the sign position is blank (20H).

7.6.4 Command Compatibility with the Model 3560 AC mΩ HiTESTER

Model 3561 and 3561-01 BATTERY HiTESTERs accept all of the commands supported by the HIOKI 3560 AC mΩ HiTESTER.
However the following differences result from the functional differences.

Comparator Tables

Up to 30 comparator settings can be saved with the Model 3560. The settings of each table can be changed directly by specifying the table number.
With this instrument, up to 126 measurement configurations (including comparator settings) can be saved (Panel Save). Settings for each configuration cannot be set directly. To recall saved configuration settings, specify the table (panel) number and execute Panel Load. A table number does not need to be specified for comparator settings.

Comparator Operations

Model 3560 judges resistance and voltage measurements together as PASS/FAIL.
This instrument judges resistance and voltage independently. Also, when the Comparator function is enabled (ON), auto-ranging is disabled (OFF).

Voltage Limiter

This instrument does not include a voltage limiter function (limiting open-terminal voltage to 20 mV). This instrument's open-terminal voltage is 7 V peak dropping to a few millivolts when the test leads are connected to a test object.

Sense Line Disconnect Detection

The sense line disconnect detection function cannot be switched on/off with this instrument. Detection is always enabled.

Resistance Value Digits with FAST Sampling

When FAST sampling is enabled on Model 3560, the number of resistance measurement digits is decreased from five to four.
With this instrument, measurement values are always five digits (31,000 counts) regardless of sampling rate.

Voltage Measurement

Model 3560 provides 5 and 50 V ranges, with five-digit (50,000 count) measurement values.
This instrument provide one 20 V range with six-digit measurement values (up to 20.0000 V, one digit more than Model 3560).

Compatibility of each of the Model 3560 commands is described below with details of the functional differences with this instrument.

Message ([ ] = optional)	Data Contents ( ) = response data	Differences Model 3561 (3561-01)	Model 3560
Standard Commands			
∗IDN?	<Manufacturer's name>,<Model name>,0, <Software version>	Model name in response data: 3561 (3561-01)	Model name in response data: 3560
∗OPC ∗OPC?	———————— 1		
∗RST	————————	Initialization contents Measurement mode: ΩV mode (Resistance and voltage measurement) Header: OFF	Initialization contents Measurement mode: Resistance measurement mode Header: ON
∗SRE ∗SRE?	0 to 255 (NR1)		
∗STB?	0 to 255 (NR1)		
∗TRG	————————		
∗TST?	0 to 3 (NR1)	Response data bit2: -, bit1: EEP-ROM, bit0: RAM	Response data bit2: EEP-ROM, bit1: RAM, bit0: ROM
∗WAI			
Device-Specific Commands			
:MODe :MODe?	R/ RV		
:RRANge :RRANge?	0 to 3E+0 300E-3/ 3E+0	Resistance range: 0 to 3.1E+0 (Although not an error, measurements are valid only within the provided 300 mΩ and 3 Ω ranges)	Resistance range: 0 to 3.1E+3
:VRANge :VRANge?	-50 to 50 20E+0	Voltage range: -20 to 20 (Although not an error, measurements are valid only) Response: 20E+0	Voltage range: -50 to 50 Response: 5E+0/ 50E+0
:AUTorange :AUTorange?	1/ 0/ ON/ OFF ON/ OFF	Setting is not possible when the comparator is enabled (when the comparator is set to ON, auto-ranging is turned OFF).	Setting is possible even when the comparator is enabled (ON).
:ADJust?	0/ 1	Performs a measurement to generate the zero-adjustment value Zero-adjustment range: 1000 counts	Applies the currently displayed value as the zero-adjustment value Zero-adjustment range: 2400 counts
:SAMPle :SAMPle?	FAST/ MEDium/ SLOW		
:COMParator :COMParator?	0 to 30	Range of panel numbers: Turns Off when the panel number is 0, and turns On when the panel number is 1 to 30 Response: Returns 0 when the comparator is disabled (OFF), and 1 when enabled (ON)	Range of Comparator Numbers: 0 to 30 Response: Returns the response number
:CSET:MODe :CSET:MODe?	R/ RV		
:CSET:NUMBer :CSET:NUMBer?	1 to 126	(function not available)	Specifies the comparator table number to set

Message ([ ] = optional)	Data Contents ( ) = response data	Differences Model 3561 (3561-01)	Model 3560
:CSET:RPARameter :CSET:RPARameter?	<Upper threshold/ Lower threshold>	Setting range: 0 to 3.1000E+0 (only valid within 300 mΩ and 3 Ω ranges)	Setting range: 0 to 3.1000E+3
:CSET:RRANge :CSET:RRANge?	0 to 3E+0 300E-3/ 3E+0	Resistance range: 0 to 3.1E+0 (Although not an error, measurements are valid only within the provided 300 mΩ and 3 Ω ranges)	Resistance range: 0 to 3.1E+3
:CSET:VPARameter :CSET:VPARameter?	<Upper threshold/ Lower threshold>	Setting range: 0 to 50.0000 (20 V range) * Negative setting values are invalid.	Setting range: -5.0000 to 5.0000 (5 V range) -50.000 to 50.000 (50 V range)
:CSET:VRANge :CSET:VRANge?	-50 to 50 20E+0	Voltage range: -20 to 20 (Although not an error, measurements are valid only Response: 20E+0	Voltage range: -50 to 50 Response: 5E+0/ 50E+0
:CTMode :CTMode?	AUTo/ MANual		
:MEASure:BATTery?	<Measured resistance, Measured voltage, Judgment result> FAIL/ PASS/ OFF/ NG	Resistance measurement values consist of five digits with FAST sampling * Numerical values do not include a decimal point.	Resistance measurement values consist of four digits with FAST sampling * Numerical values do not include a decimal point.
:MEASure:RESistance?	<Measured resistance, Judgment result> FAIL/ PASS/ OFF/ NG (ΩV) HI/ IN/ LO/ OFF/ NG (Ω)	Resistance measurement values consist of five digits with FAST sampling * Numerical values do not include a decimal point.	Resistance measurement values consist of four digits with FAST sampling * Numerical values do not include a decimal point.
:MEASure:VOLTage?	<Measured voltage, Judgment result> FAIL/ PASS/ OFF/ NG	Response: Mark: one character + six numerals (20.0000 V range) * Numerical values do not include a decimal point.	Response: * Numerical values do not include a decimal point.
:FREQuency :FREQuency?	50/60		
:LOCK:KEY :LOCK:KEY?	ON/OFF		
:HEADer :HEADer?	ON/OFF		
:LOCK:EXTernal :LOCK:EXTernal?	ON/OFF		
:CSET:BEEPer :CSET:BEEPer?	OFF/ PASS/ FAIL (ΩV) OFF/ IN/ HL (Ω)		
:HOLD :HOLD?	ON/ OFF		
:LIMit :LIMit?	ON/ OFF	(function not available)	Open terminal voltage is limited to 20 mV
:SENSecheck :SENSecheck?	ON/ OFF	(function not available)	Sense line disconnect detection is provided
:ZERoclear			

Measurement Value Formats (commands compatible with Model 3560)

For the commands that acquire measurement values (`:MEASure:BATTery?`, `:MEASure:RESistance?` and `:MEASure:VOLTage?`), the response formats are as follows.

Measured Resistance

Measurement Range	Measured Value
300 mΩ	□□□.□□E-3
3 Ω	□.□□□□E+0
± OF	1.0000E+8
Measurement Fault	1.0000E+9

Measured Voltage

Measurement Range	Measured Value
20 V	±□□.□□□□E+0
± OF	±1.0000E+8
Measurement Fault	1.0000E+9

- The positive sign for measured voltage values is returned as a space character.
- The number of displayed digits is unaffected by sampling rate.

Reference: Model 3560 Measurement Value Formats

Measured Resistance

Measurement Range	FAST	MEDIUM/ SLOW
30 mΩ	□□□.□E-3	□□□.□□E-3
300 mΩ	□□□.□E-3	□□□.□□E-3
3 Ω	□.□□□E+0	□.□□□□E+0
30 Ω	□□.□□E+0	□□.□□□E+0
300 Ω	□□□.□E+0	□□□.□□E+0
3 kΩ	□.□□□E+3	□.□□□□E+3
± OF	1.0000E+8	1.0000E+8
Measurement Fault	1.0000E+9	1.0000E+9

Measured Voltage

Measurement Range	All sampling rates
5 V	±□.□□□□E+0
50 V	±□□.□□□E+0
± OF	±1.0000E+8
Measurement Fault	1.0000E+9

7.7 Basic Data Importing Methods

Flexible data importing is available depending on the application.

Free-Run Data Importing

Initial Setup
`:INITiate:CONTinuous ON` (enable continuous measurement)
`:TRIGger:SOURce IMM` (internal triggering)

Importing
`:FETCh?`
Imports the most recent measurement

Importing by Host Triggering

Initial Setup
`:INITiate:CONTinuous OFF` (disable continuous measurement)
`:TRIGger:SOURce IMM` (internal triggering)

Importing
`:READ?`
A trigger occurs, and a measurement is taken and the result is transferred.

Importing Data by TRIG Key or $\overline{\text{TRIG}}$ Terminal

Initial Setup
`:INITiate:CONTinuous OFF` (disable continuous measurement)
`:TRIGger:SOURce EXT` (external triggering)

Importing
`:READ?`
When triggered by the **TRIG** key or TRIG terminal, a measurement is taken and the result is transferred.

7.8 Sample Programs

These sample programs are written in Microsoft Visual Basic 5.0 and 6.0.

- The following are used for communication:
  For RS-232C communication: MSComm from Visual Basic Professional
  For GP-IB communication: National Instruments GP-IB Board, Driver and Module for Visual Basic
- During communications, the terminator setting is supposed to be as follows:
  RS-232C: CR+LF
  GP-IB: LF

Visual Basic is a registered trademark of Microsoft Corporation.

RS-232C Communications

(Using Microsoft Visual Basic Professional MSComm)

(1) Simple Resistance Measurement

Imports measured values 10 times, and saves measurements in a text file.

```
Private Sub MeasureSubRS()
Dim recvstr As String                                   'Receiving char string
Dim i As Integer

MSComm1.Settings = "9600,n,8,1"                         'Comm port setting
MSComm1.PortOpen = True                                 'Open a port
Open App.Path & "\data.csv" For Output As #1            'Open a text file for saving

MSComm1.Output = ":TRIG:SOUR IMM" & vbCrLf              'Select internal triggering
MSComm1.Output = ":INIT:CONT ON" & vbCrLf               'Continuous measurement ON
For i = 1 To 10
   MSComm1.Output = ":FETCH?" & vbCrLf                  'Send ":FETCH?" to import the most recent
                                                        measurement
   recvstr = ""                                         'From here on, continue receiving until an LF code
                                                        occurs
   While Right(recvstr, 1) <> Chr(10)
      recvstr = recvstr + MSComm1.Input
      DoEvents
   Wend
   recvstr = Left(recvstr, Len(recvstr) - 2)            'Delete the terminator (CR+LF)
  Print #1, Str(i) & "," & recvstr                      'Write to the file
Next

Close #1
MSComm1.PortOpen = False
End Sub
```

(2) Measure Resistance by PC Key

Measures and imports by key input on the PC, and saves measurements in a text file.

```
Private Sub MeasureReadSubRS()
Dim recvstr As String                                   'Receiving char string
Dim i As Integer

MSComm1.Settings = "9600,n,8,1"                         'Comm port setting
MSComm1.PortOpen = True                                 'Open a port
Open App.Path & "\data.csv" For Output As #1            'Open a text file for saving

MSComm1.Output = ":TRIG:SOUR IMM" & vbCrLf              'Select internal triggering
MSComm1.Output = ":INIT:CONT OFF" & vbCrLf              'Continuous measurement OFF
For i = 1 To 10
   'Wait for PC key input
   'Create a key input check routine to set InputKey() = True when a key is pressed
   Do While 1
      If InputKey() = True Then Exit Do
      DoEvents
   Loop

   'After confirming key input, measure once, and read the measured value
   MSComm1.Output = ":READ?" & vbCrLf                   'Send ":READ?" to measure and import the
                                                        measurement
   recvstr = ""                                         'From here on, continue receiving until an LF code
                                                        occurs
   While Right(recvstr, 1) <> Chr(10)
      recvstr = recvstr + MSComm1.Input
      DoEvents
   Wend
   recvstr = Left(recvstr, Len(recvstr) - 2)            'Delete the terminator (CR+LF)
   Print #1, Str(i) & "," & recvstr                     'Write to the file
Next

Close #1
MSComm1.PortOpen = False
End Sub
```

(3) External Trigger Measurement 1

Measure and import according to external triggering of the instrument (**TRIG** key or EXT I/O TRIG terminal input), or by PC key input, and save measurements in a text file.

```
Private Sub MeasureTrigSubRS()
Dim recvstr As String                                   'Receiving char string
Dim i As Integer

MSComm1.Settings = "9600,n,8,1"                         'Comm port setting
MSComm1.PortOpen = True                                 'Open a port
Open App.Path & "\data.csv" For Output As #1            'Open a text file for saving

MSComm1.Output = ":TRIG:SOUR EXT" & vbCrLf              'Select external triggering
MSComm1.Output = ":INIT:CONT OFF" & vbCrLf              'Continuous measurement OFF
For i = 1 To 10
   MSComm1.Output = ":READ?" & vbCrLf                   'Send ":READ?" to measure and import the
                                                        measurement

   recvstr = ""                                         'From here on, continue receiving until an LF code
                                                        occurs
   While Right(recvstr, 1) <> Chr(10)
      recvstr = recvstr + MSComm1.Input
      DoEvents

      'To execute trigger measurement when a PC key is pressed,
      'Create a key input check routine to set InputKey() = True when a key is pressed
      If InputKey() = True Then
         MSComm1.Output = "*TRG" & vbCrLf               'When key input occurs, send "*TRG" to trigger
                                                        measurement
      End If
   Wend
   recvstr = Left(recvstr, Len(recvstr) - 2)            'Delete the terminator (CR+LF)
   Print #1, Str(i) & "," & recvstr                     'Write to the file
Next

Close #1
MSComm1.PortOpen = False
End Sub
```

(4) External Trigger Measurement 2

Measure and import according to external triggering of the instrument (**TRIG** key or EXT I/O TRIG terminal input), and save measurements in a text file.
(The instrument imports the most recent measurement by trigger input timing with the continuous measurement state)

```
Private Sub MeasureTrig2SubRS()
Dim recvstr As String                                   'Receiving char string
Dim i As Integer

MSComm1.Settings = "9600,n,8,1"                         'Comm port setting
MSComm1.PortOpen = True                                 'Open a port
Open App.Path & "\data.csv" For Output As #1            'Open a text file for saving

MSComm1.Output = ":TRIG:SOUR IMM" & vbCrLf              'Select internal triggering
MSComm1.Output = ":INIT:CONT ON" & vbCrLf               'Continuous measurement ON

'Clear confirmation of  External I/O TRIG input
MSComm1.Output = ":IO:IN?" & vbCrLf
recvstr = ""
While Right(recvstr, 1) <> Chr(10)
   recvstr = recvstr + MSComm1.Input
   DoEvents
Wend

For i = 1 To 10
   'Wait for External I/O TRIG input
   Do While 1
      MSComm1.Output = ":IO:IN?" & vbCrLf
      recvstr = ""
      While Right(recvstr, 1) <> Chr(10)
         recvstr = recvstr + MSComm1.Input
         DoEvents
      Wend
      If Left(recvstr, 1) = "1" Then Exit Do
      DoEvents
   Loop

   MSComm1.Output = ":FETCH?" & vbCrLf                  'Send ":FETCH?" to import the most recent
                                                        measurement

   recvstr = ""                                         'From here on, continue receiving until an LF code
                                                        occurs
   While Right(recvstr, 1) <> Chr(10)
      recvstr = recvstr + MSComm1.Input
      DoEvents
   Wend
   recvstr = Left(recvstr, Len(recvstr) - 2)            'Delete the terminator (CR+LF)
   Print #1, Str(i) & "," & recvstr                     'Write to the file
Next

Close #1
MSComm1.PortOpen = False
End Sub
```

(5) Set Measurement State

Sets up the measurement setting state.

```
'Function: ΩV
'Range: 300 mΩ
'Sampling: SLOW
'Triggering: Internal
'Comparator: ON, Beeper HL,
              Resistance  High/Low mode, Upper threshold 20000 (200.00 mΩ), Lower threshold 10000 (100.00 mΩ)
              Voltage  REF/%, Reference value 150000 (15.0000 V), toTolerance 0.1%

Private Sub SettingsSubRS()
MSComm1.Settings = "9600,n,8,1"                          'Comm port setting
MSComm1.PortOpen = True                                  'Open a port

MSComm1.Output = ":FUNC RV" & vbCrLf                     'Select ΩV mode
MSComm1.Output = ":RES:RANG 300E-3" & vbCrLf             'Select 300 mΩ range
MSComm1.Output = ":SAMP:RATE SLOW" & vbCrLf              'Select SLOW sampling
MSComm1.Output = ":TRIG:SOUR IMM" & vbCrLf               'Select internal triggering
MSComm1.Output = ":INIT:CONT ON" & vbCrLf                'Continuous measurement ON
MSComm1.Output = ":CALC:LIM:BEEP HL" & vbCrLf            'From here on, comparator settings
MSComm1.Output = ":CALC:LIM:RES:MODE HL" & vbCrLf
MSComm1.Output = ":CALC:LIM:RES:UPP 20000" & vbCrLf
MSComm1.Output = ":CALC:LIM:RES:LOW 10000" & vbCrLf
MSComm1.Output = ":CALC:LIM:VOLT:MODE REF" & vbCrLf
MSComm1.Output = ":CALC:LIM:VOLT:REF 150000" & vbCrLf
MSComm1.Output = ":CALC:LIM:VOLT:PERC 0.1" & vbCrLf
MSComm1.Output = ":CALC:LIM:STAT ON" & vbCrLf            'Comparator ON

MSComm1.PortOpen = False
End Sub
```

GP-IB Communications

(Using National Instruments GP-IB Board)

(1) Simple Resistance Measurement

Imports measured values 10 times, and saves measurements in a text file.

```
Private Sub MeasureSub()
Dim buffer As String * 40                    'Receiving butter
Dim recvstr As String                        'Receiving char string
Dim pad As Integer                           'Controller access
Dim gpibad As Integer                        'Device Address
Dim timeout As Integer                       'Timeout period
Dim ud As Integer                            'State (unused)
Dim i As Integer

pad = 0                                      'Board Address 0
gpibad = 1                                   '3561 (3561-01) Address 1
timeout = T10s                               'Timeout about 10s

Call ibfind("gpib0", 0)                      'Initialize GP-IB
Call ibdev(pad, gpibad, 0, timeout, 1, 0, ud)
Call SendIFC(pad)
Open App.Path & "\data.csv" For Output As #1 'Open a text file for saving

Call Send(pad, gpibad, ":TRIG:SOUR IMM", NLend)  'Select internal triggering
Call Send(pad, gpibad, ":INIT:CONT ON", NLend)   'Continuous measurement ON
For i = 1 To 10
   Call Send(pad, gpibad, ":FETCH?", NLend)      'Send ":FETCH?" to import the most recent
                                                 measurement
   Call Receive(pad, gpibad, buffer, STOPend)    'Receive
   recvstr = Left(buffer, InStr(1, buffer, Chr(10)) - 1)
   Print #1, Str(i) & "," & recvstr              'Write to the file
Next

Close #1
Call ibonl(pad, 0)
End Sub
```

(2) Measure Resistance by PC Key

Measures and imports by key input on the PC, and saves measurements in a text file.

```
Private Sub MeasureReadSub()
Dim buffer As String * 40                          'Receiving butter
Dim recvstr As String                              'Receiving char string
Dim pad As Integer                                 'Controller access
Dim gpibad As Integer                              'Device Address
Dim timeout As Integer                             'Timeout period
Dim ud As Integer                                  'State (unused)
Dim i As Integer

pad = 0                                            'Board Address 0
gpibad = 1                                         '3561 (3561-01) Address 1
timeout = T10s                                     'Timeout about 10s

Call ibfind("gpib0", 0)                            'Initialize GP-IB
Call ibdev(pad, gpibad, 0, timeout, 1, 0, ud)
Call SendIFC(pad)
Open App.Path & "\data.csv" For Output As #1       'Open a text file for saving

Call Send(pad, gpibad, ":TRIG:SOUR IMM", NLend)    'Select internal triggering
CCall Send(pad, gpibad, ":INIT:CONT OFF", NLend)   'Continuous measurement OFF
For i = 1 To 10
   'Wait for PC key input
   'Create a key input check routine to set InputKey() = True when a key is pressed
   Do While 1
      If InputKey() = True Then Exit Do
      DoEvents
   Loop

   'After confirming key input, measure once, and read the measured value
   Call Send(pad, gpibad, ":READ?", NLend)         'Send ":READ?" to measure and import the
                                                   measurement
   Call Receive(pad, gpibad, buffer, STOPend)      'Receive
   recvstr = Left(buffer, InStr(1, buffer, Chr(10)) - 1)
   Print #1, Str(i) & "," & recvstr                'Write to the file
Next

Close #1
Call ibonl(pad, 0)
End Sub
```

(3) External Trigger Measurement 1

Measure and import according to external triggering of the instrument (**TRIG** key or EXT I/O TRIG terminal input), and save measurements in a text file.

```
Private Sub MeasureTrigSub()
Dim buffer As String * 40                    'Receiving butter
Dim recvstr As String                        'Receiving char string
Dim pad As Integer                           'Controller access
Dim gpibad As Integer                        'Device Address
Dim timeout As Integer                       'Timeout period
Dim ud As Integer                            'State (unused)
im i As Integer

pad = 0                                      'Board Address 0
gpibad = 1                                   '3561 (3561-01) Address 1
timeout = T100s                              'Timeout 100s (because of external trigger wait state)

Call ibfind("gpib0", 0)                      'Initialize GP-IB
Call ibdev(pad, gpibad, 0, timeout, 1, 0, ud)
Call SendIFC(pad)
Open App.Path & "\data.csv" For Output As #1 'Open a text file for saving

Call Send(pad, gpibad, ":TRIG:SOUR EXT", NLend)  'Select external triggering
Call Send(pad, gpibad, ":INIT:CONT OFF", NLend)  'Continuous measurement OFF
For i = 1 To 10
   Call Send(pad, gpibad, ":READ?", NLend)   'Send ":READ?" to measure and import the
                                             measurement
   Call Receive(pad, gpibad, buffer, STOPend)  'Receive
   recvstr = Left(buffer, InStr(1, buffer, Chr(10)) - 1)
   Print #1, Str(i) & "," & recvstr          'Write to the file
Next

Close #1
Call ibonl(pad, 0)
End Sub
```

(4) External Trigger Measurement 2

Measure and import according to external triggering of the instrument (**TRIG** key or EXT I/O TRIG terminal input), and save measurements in a text file.
(The instrument imports the most recent measurement by trigger input timing with the continuous measurement state)

```
Private Sub MeasureTrig2Sub()
Dim buffer As String * 40                    'Receiving butter
Dim recvstr As String                        'Receiving char string
Dim pad As Integer                           'Controller access
Dim gpibad As Integer                        'Device Address
Dim timeout As Integer                       'Timeout period
Dim ud As Integer                            'State (unused)
Dim i As Integer

pad = 0                                      'Board Address 0
gpibad = 1                                   '3561 (3561-01) Address 1
timeout = T100s                              'Timeout 100s (because of external trigger wait state)

Call ibfind("gpib0", 0)                      ' Initialize GP-IB
Call ibdev(pad, gpibad, 0, timeout, 1, 0, ud)
Call SendIFC(pad)
Open App.Path & "\data.csv" For Output As #1 'Open a text file for saving

Call Send(pad, gpibad, ":TRIG:SOUR IMM", NLend)  'Select internal triggering
Call Send(pad, gpibad, ":INIT:CONT ON", NLend)   'Continuous measurement ON

   'Clear confirmation of  External I/O TRIG input
Call Send(pad, gpibad, ":IO:IN?", NLend)
Call Receive(pad, gpibad, buffer, STOPend)
recvstr = Left(buffer, InStr(1, buffer, Chr(10)) - 1)
For i = 1 To 10
   'Wait for External I/O TRIG input
   Do While 1
      Call Send(pad, gpibad, ":IO:IN?", NLend)
      Call Receive(pad, gpibad, buffer, STOPend)
      If Left(buffer, 1) = "1" Then Exit Do
      DoEvents
   Loop

   Call Send(pad, gpibad, ":FETCH?", NLend)  'Send ":FETCH?" to import the most recent
                                             measurement
   Call Receive(pad, gpibad, buffer, STOPend)  'Receive
   recvstr = Left(buffer, InStr(1, buffer, Chr(10)) - 1)
   Print #1, Str(i) & "," & recvstr           'Write to the file
Next

Close #1
Call ibonl(pad, 0)
End Sub
```

(5) Set Measurement State

Sets up the measurement setting state.

```
'Function: ΩV
'Range: 300 mΩ
'Sampling: SLOW
'Triggering: Internal
'Comparator: ON, Beeper HL,
Resistance  High/Low mode, Upper threshold 20000 (200.00 mΩ), Lower threshold 10000 (100.00 mΩ)
Voltage  REF/%, Reference value 150000 (15.0000 V), toTolerance 0.1%

Private Sub SettingsSub()
Dim pad As Integer                                  'Controller access
Dim gpibad As Integer                               'Device Address
Dim timeout As Integer                              'Timeout period
Dim ud As Integer                                   'State (unused)

pad = 0                                             'Board Address 0
gpibad = 1                                          '3561 (3561-01) Address 1
timeout = T10s                                      'Timeout about 10s

Call ibfind("gpib0", 0)                             'Initialize GP-IB
Call ibdev(pad, gpibad, 0, timeout, 1, 0, ud)
Call SendIFC(pad)

Call Send(pad, gpibad, ":FUNC RV", NLend)           'Select ΩV mode
Call Send(pad, gpibad, ":RES:RANG 300E-3", NLend)   'Select 300 mΩ range
Call Send(pad, gpibad, ":SAMP:RATE SLOW", NLend)    'Select SLOW sampling
Call Send(pad, gpibad, ":TRIG:SOUR IMM", NLend)     'Select internal triggering
Call Send(pad, gpibad, ":INIT:CONT OFF", NLend)     'Continuous measurement OFF
Call Send(pad, gpibad, ":CALC:LIM:BEEP HL", NLend)  'From here on, comparator settings
Call Send(pad, gpibad, ":CALC:LIM:RES:MODE HL", NLend)
Call Send(pad, gpibad, ":CALC:LIM:RES:UPP 20000", NLend)
Call Send(pad, gpibad, ":CALC:LIM:RES:LOW 10000", NLend)
Call Send(pad, gpibad, ":CALC:LIM:VOLT:MODE REF", NLend)
Call Send(pad, gpibad, ":CALC:LIM:VOLT:REF 150000", NLend)
Call Send(pad, gpibad, ":CALC:LIM:VOLT:PERC 0.1", NLend)
Call Send(pad, gpibad, ":CALC:LIM:STAT ON", NLend)  'Comparator ON

Call ibonl(pad, 0)
End Sub
```

Specifications Chapter 8

8.1 Basic Specifications

Measurement Items

Measurement items	Resistance and voltage	
Resistance measurement method	AC four-terminal method	
Measurement current frequency	1 kHz	
Resistance measurement range	0.01 mΩ to 3.1 Ω	
Voltage measurement range	± 0.1 mV DC to ± 19.9999 V DC	
Measurement modes	• ΩV mode • Ω mode • V mode	(Resistance and voltage measurement) (Resistance measurement) (Voltage measurement)
Maximum input voltage	± 22 V DC	
Maximum rated voltage to earth	± 70 V DC	
Input impedance	Approx. 1 MΩ	

Measurement Ranges

Resistance measurement	300 mΩ/ 3 Ω
Voltage measurement	20 V

Measurement Value Display

Maximum displayed count	Resistance measurement : “31000” Voltage measurement : “199999”
Overflow display	Resistance measurement: OF indicates a measurement exceeds 31000 (display counts) -OF indicates a measurement is below -1000 Voltage measurement: OF indicates a measurement exceeds 199999 (display counts) -OF indicates a measurement is below -199999
Measurement fault detection	”- - - - -”

Sampling Time

Sampling rate	EX.FAST/ FAST/ MEDIUM/ SLOW (four steps)
Sampling time	

Sampling	EX.FAST	FAST	MEDIUM	SLOW
ΩV (50 Hz) (60 Hz)	7 ms	23 ms	83 ms 69 ms	258 ms 252 ms
Ω (50 Hz) (60 Hz)	4 ms	12 ms	42 ms 35 ms	157 ms 150 ms
V (50Hz) (60Hz)	4 ms	12 ms	42 ms 35 ms	157 ms 150 ms

* Tolerance for SLOW sampling is ± 5 ms, and ± 1 ms for other sampling rates
* Values within parentheses are line frequency settings

Response Time

Response time	Response time is specified as the interval from the moment of connecting (open-circuit) test leads to a test object until the signal becomes stable within the measurement accuracy of the internal measurement circuitry. Resistance measurement : Approx. 3 ms Voltage measurement : Approx. 3 ms * Response times are nominal values. Actual values depend on the impedance characteristics of the object being measured.
Total measurement time	Overall time required for measurement: Response time + sampling time

Zero-Adjustment

Zero-adjustment function	• Zero-adjustment setting ON/ OFF (Common to both resistance and voltage) • Zero-adjustment clear Turns zero-adjustment off and clears all zero-adjustment offset data
Zero-adjustment range	Resistance measurement : -1000 to 1000 count Voltage measurement : -1000 to 1000 count

Self-Calibration

Calibration mode	AUTO/ MANUAL
AUTO	Executes automatically once every 30 minutes
MANUAL	Executes manually by EXT I/O signal or remote command

* When SLOW sampling is selected, self-calibration is performed upon each measurement. In this state, the calibration mode setting is ignored.

Trigger

Trigger source	Internal/ External

Delay

Delay function	ON/ OFF
Delay time	0 to 9.999 sec

Averaging

Averaging function	ON/ OFF
No. of samples to average	2 to 16
Averaging	Moving average with internal triggering, and simple average with external triggering

Comparator

Comparator function	ON/ OFF (Common to both resistance and voltage)
Comparator setting	• Comparator threshold method Upper and lower threshold/ Reference value and tolerance Upper and lower threshold: 0 to 99999 (Resistance) / 0 to 999999 (Voltage) • Reference value and tolerance: 0 to 99999 (Resistance) / 0 to 999999 (Voltage) %: 0.000% to 99.999% • Comparator judgment beeper OFF/ HL/ IN/ BOTH1/ BOTH2 • Comparator execution mode AUTO/ MANUAL * Measurement value data and statistical 3σ (population standard deviation X 3) can be set automatically.
Decision	Judgment result: Hi/ IN/ Lo (resistance and voltage judged independently) AND judgment: Calculates the logical AND of resistance and voltage judgment results Measurement fault value judgments: OF Hi judgment -OF Lo judgment Measurement faultNot judged (no judgment result)

Statistical Calculation

Statistical calculation	ON/ OFF/ clear Auto-clear after printing statistical data
Calculations	Total data counts, Valid data counts, Maximum, Minimum, Mean, Standard deviation, Population standard deviation and Process capability indices (Cp and CpK)
Calculations trigger	Statistical calculation of measured values initiated by EXT I/O signals, key or remote command

Measurement Memory and Batch Download Functions

Measurement memory	ON/ OFF/ clear
Memory trigger	Up to 400 measurement values can be stored in internal memory by EXT I/O signals, key or remote command. Stored measurement values can be batch downloaded by remote command.

Key-Lock

Key-lock	ON/ OFF Key operations are disabled when ON.

Panel Save

Panel save function	Measurement configurations can be saved and reloaded by specifying a Panel number
No. of panel to save	126
Saved settings	Measurement mode, Resistance measurement range, Auto-ranging setting, Zero-adjust on/off setting and value, Sampling rate, Switching display setting, Trigger source, Delay setting, Averaging setting, Comparator setting, Statistical calculation setting and Key-lock setting

Reset

Reset	Reset/ System reset * System Reset also initializes Panel Save data

Display Device

Display device	LED

External Interfaces

EXT I/O	Input : CMOS level Output : Open collector, 35 V, 50 mA max. Input signals : Measurement start trigger, print, zero-adjustment, calibration, manual comparator and panel load (7 bit) Output signals : End-of-measurement, End measurement, Comparator result (resistance Hi/ IN/ Lo, voltage Hi/ IN/ L, AND), measurement fault and General-Purpose output (10 bit) * EXT I/O control (input) can be disabled by a remote command
RS-232C	Communications settings: Data length (8 bit), stop bit (1 bit), parity (none) Baud rate : 9600 bps/ 19200 bps/ 38400 bps Flow control : none
Printer	Output to printer via RS-232C (multi-use) Printer : Model 9670 (option) Communications settings: Data length (8 bit), stop bit (1 bit), parity (none) Baud rate : 9600 bps
GP-IB (Model 3561-01 only)	Applicable GP-IB Standards: IEEE488.2 Address : 0 to 30 Delimiter : LF/ CR+LF

8.2 Accuracy

Guaranteed Accuracy Conditions

Temperature and humidity range for guaranteed accuracy	23 ± 5°C (73 ± 9°F), 80% RH or less (non-condensating)
Zero-adjustment	After zero adjustment
Warm-up time	At least 30 minutes
Self calibration	Except when using SLOW sampling, self-calibration should be executed after warm-up. Ambient temperature after self-calibration should be maintained within ± 2°C.

Resistance Measurement

Range	300 mΩ	3 Ω
Maximum displayed values	310.00 mΩ	3.1000 Ω
Resolution	0.01 mΩ	0.1 mΩ
Measured current	10 mA ± 10%	1 mA ± 10%
Measured current frequency	1 kHz ± 0.2 Hz	
Accuracy*1	± 0.5%rdg. ± 5dgt.	
Temperature coefficient	(± 0.05%rdg. ± 0.5dgt.)/°C	
Open-terminal voltage	7 V peak	

Voltage Measurement

Range	20 V
Maximum displayed values	± 19.9999 V
Resolution	0.1 mV
Accuracy*2	± 0.01%rdg. ± 3dgt.
Temperature coefficient	(± 0.001%rdg. ± 0.3dgt.)/°C

*1: Add ± 3 dgt for EX.FAST, or ± 2 dgt for FAST and MEDIUM sampling rates.

*2: Add ± 3 dgt for EX.FAST, or ± 2 dgt for FAST and MEDIUM sampling rates.

8.3 General Specifications

Operating temperature and humidity	0 to 40°C (32 ± 104°F), 80%RH or less (non-condensating)
Storage temperature and humidity	-10 to 50°C (14 ± 122°F), 80%RH or less (non-condensating)
Temperature and humidity range for guaranteed accuracy	23 ± 5°C (73 ± 9°F), 80%RH or less (non-condensating)
Period of guaranteed accuracy	1 year
Operating environment	Indoors, Up to 2000 m (6562 ft) ASL
Rated supply voltage	AC100 V to AC240 V (Auto selecting) (Voltage fluctuations of ±10% from the rated supply voltage are taken into account.)
Rated supply frequency	50 Hz/ 60 Hz
Power consumption	30 VA
Dielectric strength	1.69 kV AC for 15s, Cutoff current 10 mA, between all power terminals and protective ground
Dimensions	Approx. 215W X 80H X 295D mm (8.46"W X 3.15"H X 11.61"D) (sans protrusions)
Mass	Approx. 2.4 kg (84.7 oz.)
Accessories	Instruction Manual..... 1 Power Cord..... 1
Options	Model 9287-10 CLIP TYPE LEAD Model 9452 CLIP TYPE LEAD Model 9453 FOUR TERMINAL LEAD Model 9455 PIN TYPE LEAD (for ultra precision) Model 9467 LARGE CLIP TYPE LEAD Model 9770 PIN TYPE LEAD Model 9771 PIN TYPE LEAD Model 9637 RS-232C CABLE (9-pin to 9-pin, crossover) Model 9638 RS-232C CABLE (9-pin to 25-pin, crossover) Model 9151-02 GP-IB CONNECTOR CABLE (2 m) Model 9151-04 GP-IB CONNECTOR CABLE (4 m) Model 9670 PRINTER (Sanei Electric Model BL-80RS II) Model 9671 AC ADAPTER (for 9670, Sanei Electric Model BL-100W) Model 9672 BATTERY PACK (for the 9670) Model 9673 BATTERY CHARGER (for the 9672) Model 9237 RECORDING PAPER (80 mm X 25 m, 4 rolls, for the 9670)
Applicable Standards	Safety EN61010-1:2001 EMC EN61326:1997+A1:1998+A2:2001+A3:2003 ClassA EN61000-3-2:2000 EN61000-3-3:1995+A1:2001
Effect of radiated radio-frequency electromagnetic field	Resistance measurement : ± 10%rdg. ± 3,000 dgt. at 10 V/m Voltage measurement : ± 0.01%rdg. ± 50 dgt. at 10 V/m
Effect of conducted radio-frequency electromagnetic field	Resistance measurement : ± 0.5%rdg. ± 100 dgt. at 3 V

Chapter 9 Maintenance and Service

9.1 Troubleshooting

- If damage is suspected, check the "Troubleshooting" section before contacting your dealer or Hioki representative.
- The fuse is housed in the power unit of the instrument. If the power does not turn on, the fuse may be blown. If this occurs, a replacement or repair cannot be performed by customers. Please contact your dealer or Hioki representative.
- Pack the instrument so that it will not sustain damage during shipping, and include a description of existing damage. We cannot accept responsibility for damage incurred during shipping.

⚠CAUTION

Calibration and repair of this instrument should be performed only under the supervision of qualified technicians knowledgeable about the dangers involved.

NOTE

If no measurement value is displayed even when the probes are shorted together, an internal fuse may have blown.
If the fuse blows, do not attempt to replace the fuse or repair the instrument: contact your dealer or Hioki representative.

Before returning for repair.

Symptom	Check Items	Countermeasure
The display does not appear when you turn the power on.	Is the power cord disconnected?	Reconnect the power cord.
Keys do not operate.	Is the unit in the key-locked state?	Disable the key-lock state. ❖See Section 4.6 Key-Lock Function (page 60).
	Is the instrument being remotely controlled externally using GP-IB?	Set GP-IB to local.
	Is the instrument being remotely controlled externally using RS-232C?	Set RS-232C to local.
An error is displayed.		❖See Section 9.3 Error Display (page 164).
Operation is abnormal.		External electrical noise may occasionally cause malfunctions. If operation seems abnormal, try executing a Reset. ❖See Section 4.12 Reset Function (page 66).

9.2 Cleaning

To clean the instrument, wipe it gently with a soft cloth moistened with water or mild detergent. Never use solvents such as benzene, alcohol, acetone, ether, ketones, thinners or gasoline, as they can deform and discolor the case.

9.3 Error Display

Display		Description
Err02	Zero-Adjust Range Error	The value before zero-adjustment exceeded 1,000 dgt.
Err10	Execution Error	The data portion of a remote command is invalid.
Err11	Command Error	The command portion of a remote command is invalid.
Err90	ROM Error	An internal program error occurred. Repair is required.
Err91	RAM Error	An internal RAM error occurred. Repair is required.
Err92	EEPROM (Adjustment Data) Error	Adjustment data is corrupted. Repair is required.
Err95	A/D Communications Error	The A/D converter is damaged. Repair is required.
- - - - -	This indicates a measurement fault. It appears in cases of a disconnected test lead, poor probe contact or when the test object's measured value is far above the measurement range. The measurement fault signal is output from the ERR terminal of the EXT I/O connector. The following causes should be considered: • A test lead may not be connected to the test object • Test object resistance may be too large for the measurement range Example: Measuring 30 Ω with the 300 mΩ range • Any of the SOURCE-H, SOURCE-L, SENSE-H or SENSE-L leads may be disconnected or poorly connected • When resistance between SOURCE-H and SOURCE-L is 50 Ω or more in the 300 mΩ range (500 Ω or more in the 3 Ω range) • Resistance between SENSE-H and SENSE-L is about 20 Ω or more (however, if test lead capacitance is more than 1 nF, measurement faults may not be detected) • The contact failure circuit protection fuse may have blown due to test lead damage, excessive wear, or impurities.	

Appendix

Appendix 1 Precautions for Making Custom Test Leads

Bear the following in mind when making custom test leads.

- Be sure to twist together the SOURCE-H and L leads, and the SENSE-H and L leads. Also, connect the shields of all leads to the SOURCE-L lead.

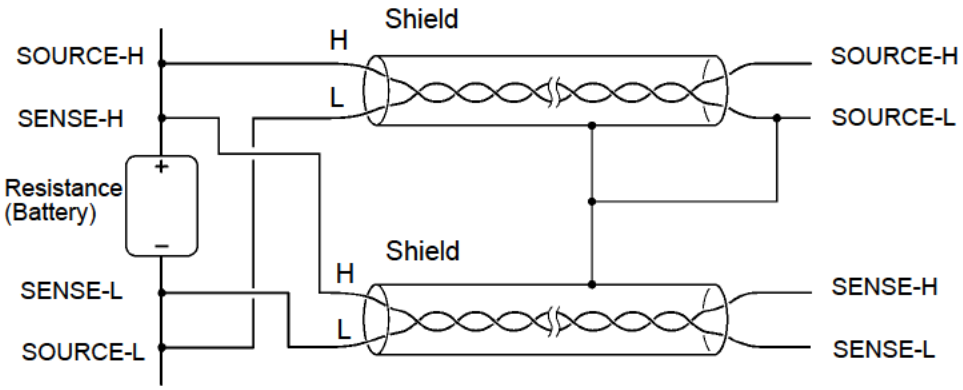

- The four-terminal design requires that all four terminals be used for measurement. Attempting to measure with two terminals (the two lines in the middle) may result in unstable or inconsistent measurements due to the effects of test lead contact resistance.

Wrong Connection

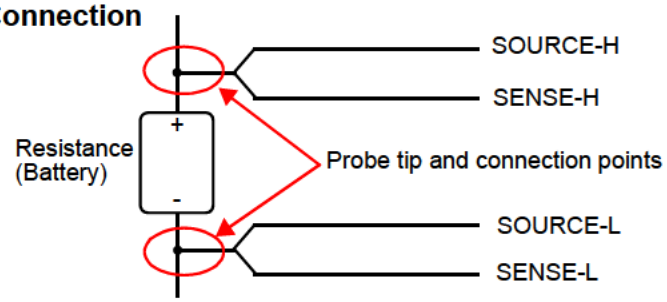

APP

- When connecting to a test object, connect SOURCE-H and SOURCE-L toward the outside, and SENSE-H and SENSE-L toward the inside.

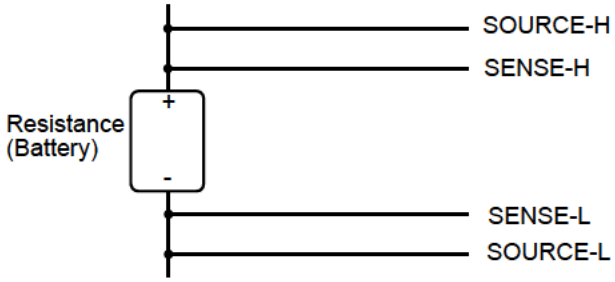

- Do not allow the test leads near metal surfaces. In particular, the lead portions that are not twisted together must be kept away from conductors to avoid unstable measurements resulting from the effects of induced current.
❖See Appendix 5 Effect of Eddy Currents (Page 170).

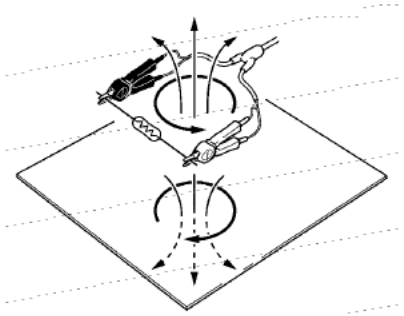

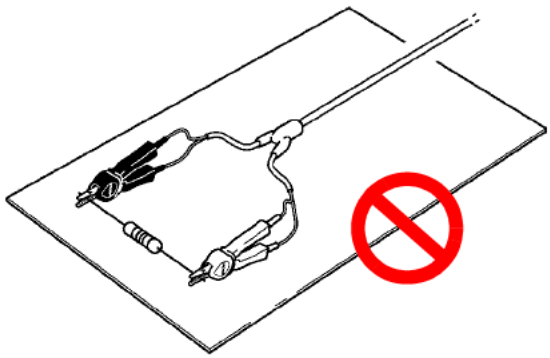

- Leads should be as short as possible (and in no case more than 5 m). Long leads are more susceptible to noise ingress and unstable measurements. The total lead resistance in both directions plus test lead contact resistance must not exceed 20 Ω.

NOTE When using the probe tips of optional separate test leads, be careful to avoid touching the shield conductors of the SOURCE-H, SENSE-H and SENSE-L lines to their center conductors.

Appendix 2 AC Four-terminal Method

The instrument uses the AC four-terminal method, so that resistance measurement can be carried out with the resistance of the leads and the contact resistance between the leads and the object to be measured canceled out. The following figure shows the principle of the AC four-terminal measurement method.

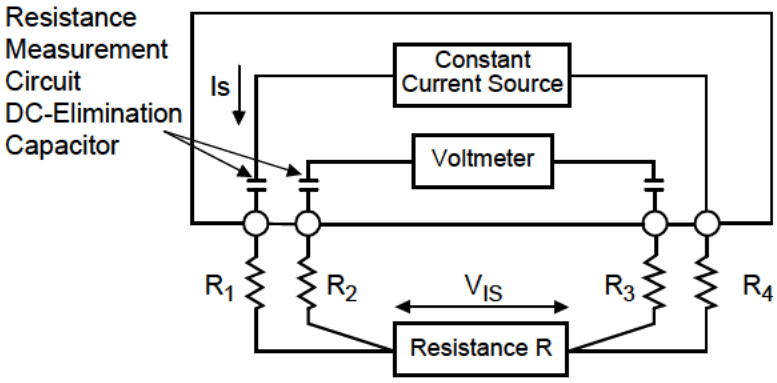

Values R1 to R4 are the resistances of the test leads plus contact resistances.

An AC current (I_s) is supplied from the SOURCE terminals of the instrument across the tested battery. The voltage drop across the internal impedance of the battery (V_{IS}) is measured by the SENSE terminals. At this point, since the SENSE terminals are connected to an internal voltmeter with a high impedance, almost no current flows through the resistances R_2 and R_3 which represent the lead resistances and contact resistances. As a result, there is almost no voltage drop across the resistances R_2 and R_3. Thus the voltage drop due to the lead resistances and contact resistances is very small, and these can be canceled out. In the instrument, a synchronized wave detection system is used, whereby the internal impedance is separated into resistance and reactance, and the resistive component only displayed.

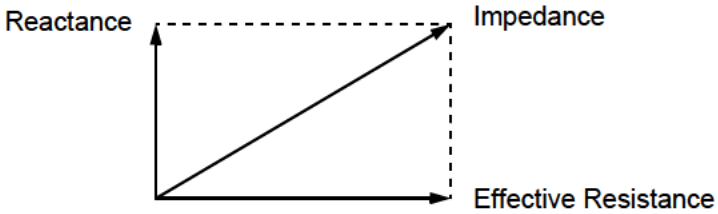

If the lead resistance, the contact resistance between measured object and lead, or the contact resistance between the lead and the instrument instrument increases, the instrument can no longer supply normal current to the measured object, resulting in an abnormal measurement status indicated by "- - - - -" within the measured resistance field. For more information on abnormal measurements, see Section 3.7.1 Measurement Fault Detection (Page 32)."

Appendix 3 Synchronous Detection System

The figure below shows an equivalent circuit for a battery. If the measured object exhibits other electrical characteristics in addition to resistance, as shown in this figure, we can use the synchronous detection system to obtain the effective resistance of the object. This synchronous detection system is also used to separate faint signals from noise.

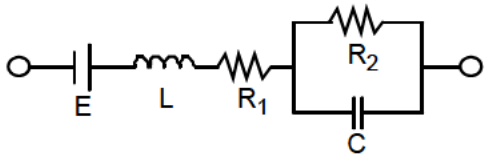

The synchronous detection system picks up the reference signal and those signals having the same phase components. The figure below gives a simplified schematic diagram of the synchronous detection system. The system consists of a multiplying circuit that multiplies two signals and a low-pass filter (LPF) that picks up only DC components from the output.

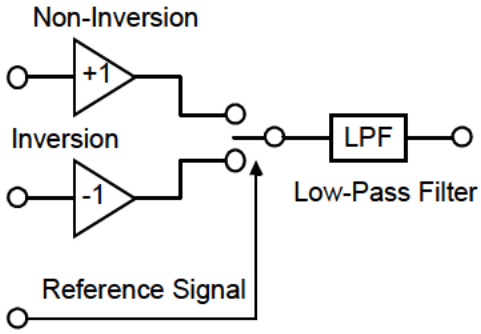

Given "v1," a reference signal voltage for the AC current generated in the instrument, and "v2," the signal voltage for use in synchronous detection, these parameters may be expressed by the equation given below. θ of v2 shows the phase difference against v1 and is generated by the reactance.

$v1 = A\sin\omega t$

$v2 = B\sin(\omega t + \theta)$

When synchronous detection is applied to both v1 and v2, they are expressed as follows:

$v1 \times v2 = 1/2AB\cos\theta - 1/2AB\cos(2\omega t + \theta)$

The first term indicates effective resistance. The second term is attenuated by the LPF. The instrument displays the first term.

Appendix 4 Configuration and Extension of the Test Leads

The test lead extension is normally performed by Hioki. If you want extension performed, contact your dealer or Hioki representative.
Observe the following points when extending test leads:

- Use the thickest lead available. Extend the lead only by the necessary amount.
- Maintain the AC four-terminal configuration while extending the lead. Changing the four-terminal configuration to a two-terminal configuration can result in measurement data being affected by lead resistance and/or contact resistance, resulting in inaccurate measurement.
- Make the branch section as short as possible. Try to extend the thick lead instead.
- Make sure the lead is insulated.
- While measuring, avoid as much as possible pulling or repositioning the test leads after executing zero adjustment.
- Extending test leads may result in excessive voltage drop. The total resistance of the test leads and contacts must remain below 20 Ω.
- To prevent eddy currents from affecting measurement, keep test leads away from metallic parts.
- After extending the test leads, confirm proper measurement operation and accuracy.

Reducing Induced Voltage

Since the instrument measures a minute resistance with AC power, it is affected by induced voltage. Induced voltage refers to voltage that allows the current generated in the instrument to build an inductive coupling in a lead and affect signal lines. Since the phase of the induced voltage is shifted from that of the AC current (reference signal) by 90 degrees, it can be eliminated with the synchronous detection circuit if the voltage is low. But for high levels, the induced voltage distorts the signals, causing incorrect synchronous detection. The instrument monitors induced voltage internally and generates an abnormal measurement signal if the level rises above a certain level. Reducing the length of the lead will lower induced voltage. Reducing the length of the branched section is particularly effective.

Appendix 5 Effect of Eddy Currents

The AC current generated in the instrument induces eddy currents in the surrounding metallic plates, which generate induced voltage in the test lead. Since the phase of this induced voltage is shifted from that of the AC current (reference signal) by 180 degrees, it cannot be eliminated by the synchronous detection circuit, resulting in measurement errors. The influence of eddy currents is a phenomenon unique to ohmmeters that measure resistance with AC power. To protect the test lead from such effects, keep metallic parts, including metallic plates, at a suitable distance from the test lead (branched section).

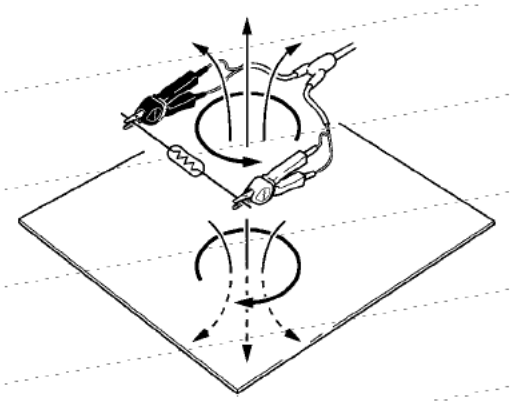

Appendix 6 Calibration Procedure

For the calibration environment, see Section Chapter 8 Specifications (Page 157)."

Calibration of the Ohmmeter

- Use the 9453 FOUR TERMINAL LEAD as the connection lead.
- Use standard resistors with excellent temperature characteristics that resist deterioration over time.
- To prevent influence by the lead, use four-terminal resistors.
- Use a resistor that will reflect the correct resistance at 1 kHz. With wire-wound resistors, the inductance element is so large that the pure resistance (DC resistance) does not equal the effective resistance (real part of impedance, displayed on the instrument).
- For connection of a standard resistor to the instrument, see the figure below.

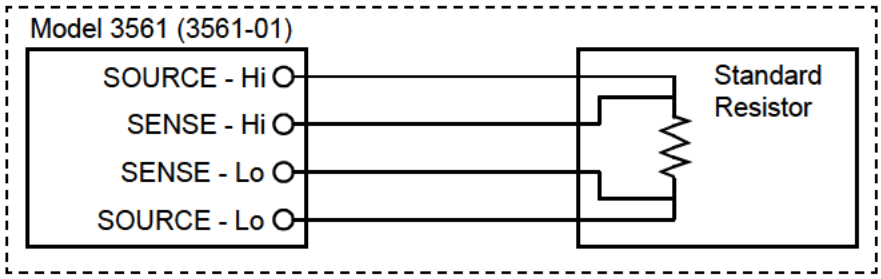

Calibration of the Voltmeter

- Use the 9453 FOUR TERMINAL LEAD as the connection lead.
- Use a generator that can output a DC voltage of 20 V.
- For connection of a generator to the instrument, see the figure below.
- Do not apply an alternating current from the instrument to the generator, as the generator may malfunction.
- Use a low-impedance voltage source.

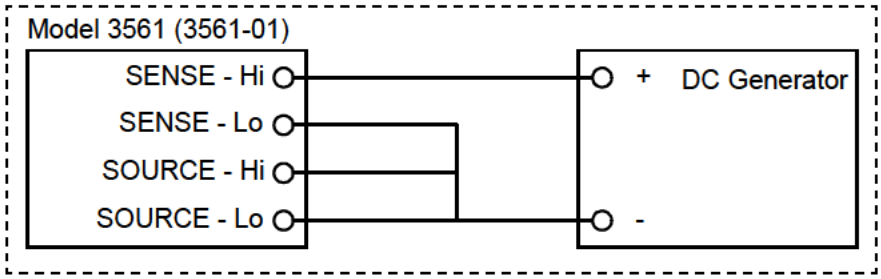

Appendix 7 Test Lead Options

Model 9287-10 CLIP TYPE LEAD

These leads have clip tips. Four-terminal measurements are provided just by clipping on to the test object.
Maximum clip diameter: 8 mm

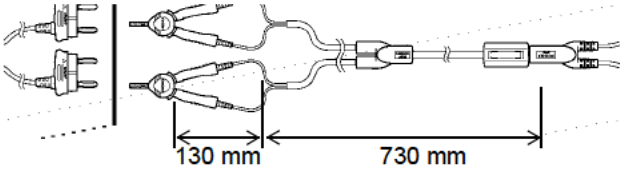

Model 9452 CLIP TYPE LEAD

The probes have pincer-type tips.
Allows reliable four-terminal measurements even on test objects with small contacts such as relay terminals and connectors.
Bifurcation-to-probe length: approx. 200 mm
Plug-to-bifurcation length: approx. 800 mm

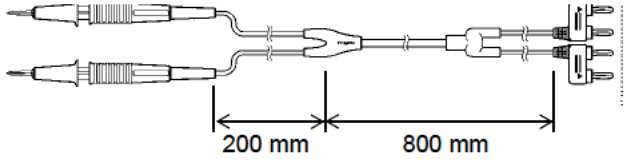

Model 9453 FOUR TERMINAL LEAD

The SOURCE leads of this four-terminal lead set have covered alligator clips, and the SENSE leads have standard test probes. Use for measuring printed circuit board pattern resistance, and where SOURCE and SENSE leads need to be connected separately.
Bifurcation-to-probe length: approx. 300 mm
Plug-to-bifurcation length: approx. 800 mm

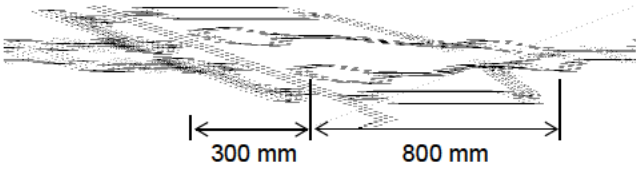

Model 9455 PIN TYPE LEAD

The probe tips have a four-terminal structure designed for checking for floating IC leads on printed circuit boards. Correct measurements are obtained even with very small test objects.
Bifurcation-to-probe length: approx. 250 mm
Plug-to-bifurcation length: approx. 400 mm

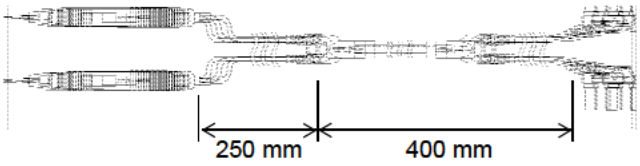

Model 9467 LARGE CLIP TYPE LEAD

These leads are designed to attach to test object with large diameter contacts. Four-terminal measurements can be made just by clipping.
Bifurcation-to-probe length: approx. 250 mm
Plug-to-bifurcation length: approx. 850 mm
Maximum clip diameter: approx. 29 mm

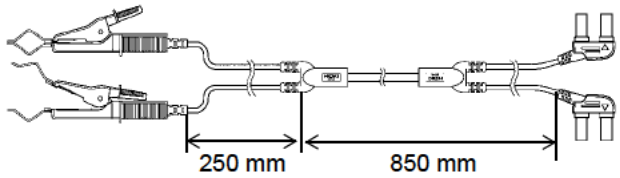

Model 9770 PIN TYPE LEAD

Even on flat contact points that cannot be clipped to, or on test objects with small contacts such as relay terminals or connectors, four-terminal measurements are available by just pressing.
Bifurcation-to-probe length: approx.250 mm
Plug-to-bifurcation length: approx.400 mm
Pin base: ϕ 1.8 mm

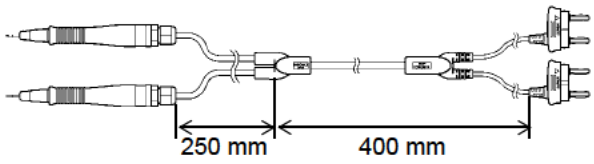

Model 9771 PIN TYPE LEAD

The tips have a four-terminal design developed for floating-foot testing of ICs mounted on boards. Resistance can be correctly measured even with small test objects.
Bifurcation-to-probe length: approx. 250 mm
Plug-to-bifurcation length: approx.400 mm
Between pin bases: 0.2 mm

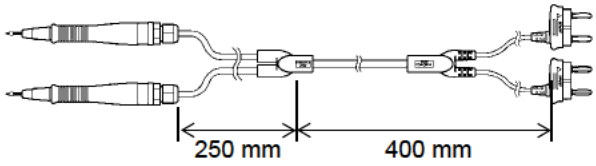

Appendix 8 Rack Mounting

By removing the screws on the sides, this instrument can be installed in a rack mounting plate.

⚠WARNING

Observe the following precautions regarding the mounting screws to avoid instrument damage and electric shock accidents.

- **When installing the Rack Mounting Plate, the screws must not intrude more than 6 mm into either side of the instrument.**
- **When removing the Rack Mounting Plate to return the instrument to stand-alone use, replace the same screws that were installed originally. (Feet: M3 x 6 mm, Sides: M4 x 6 mm)**

Rack Mounting Plate Template Diagram and Installation Procedure

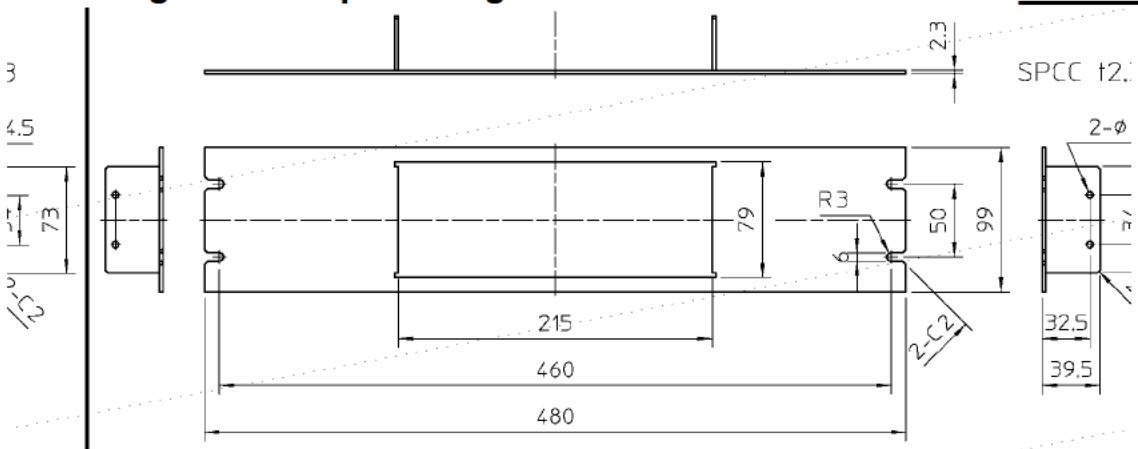

Rack Mounting Plate (JIS)

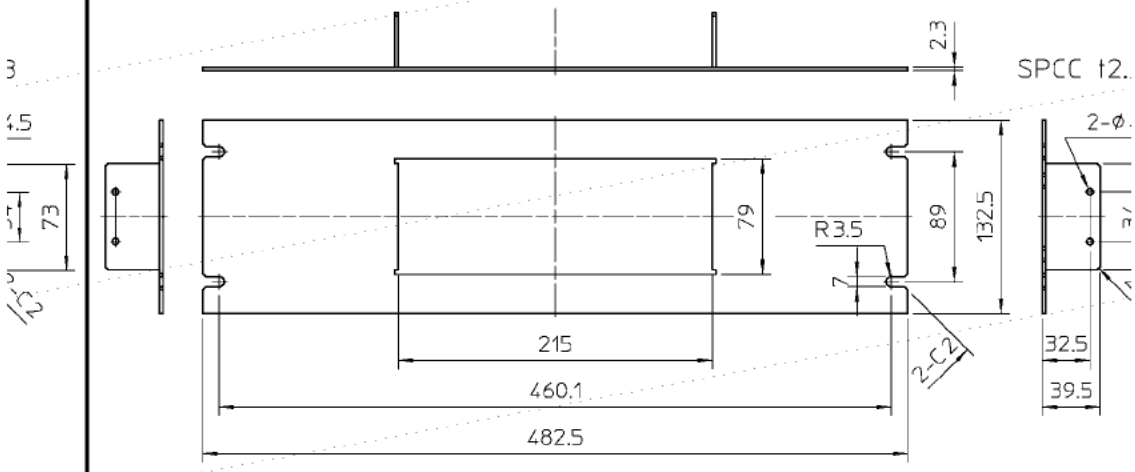

Rack Mounting Plate (EIA)

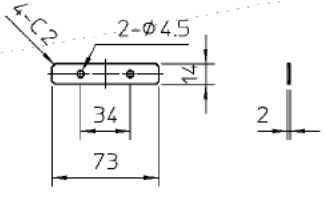

Spacer (Two Required)

APP

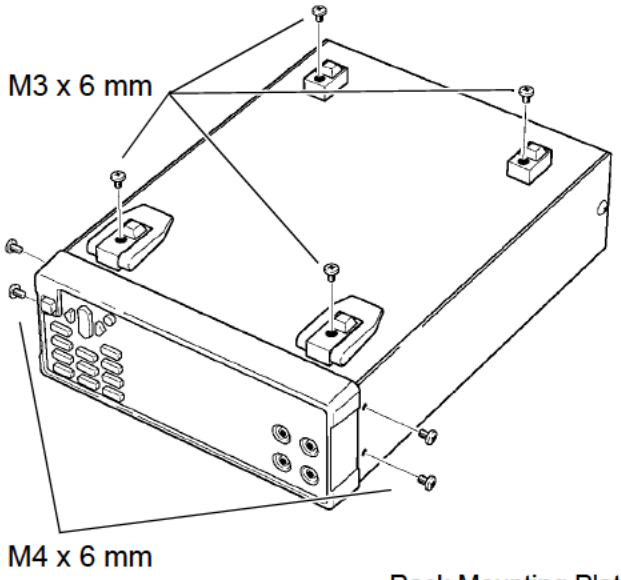

1. **Remove the feed from the bottom of the instrument, and the screws from the sides (four near the front).**

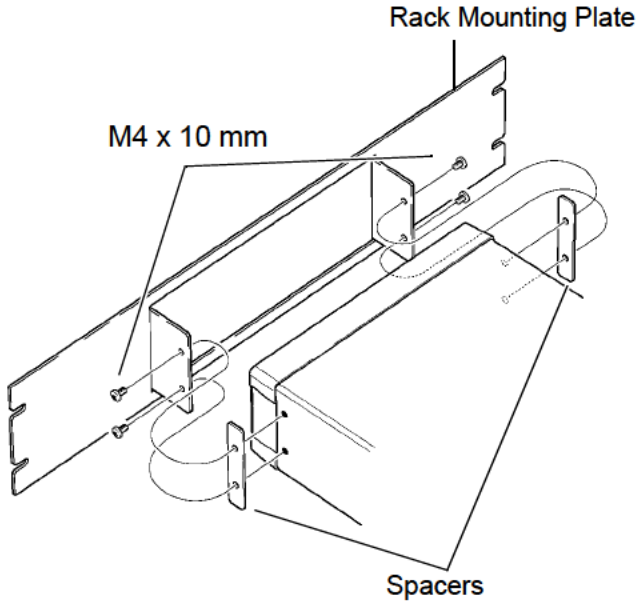

2. **Installing the spacers on both sides of the instrument, affix the Rack Mounting Plate with the M4 x 10 mm screws.**

When installing into the rack, reinforce the installation with a commercially available support stand.

Appendix 9 Dimensional Diagram

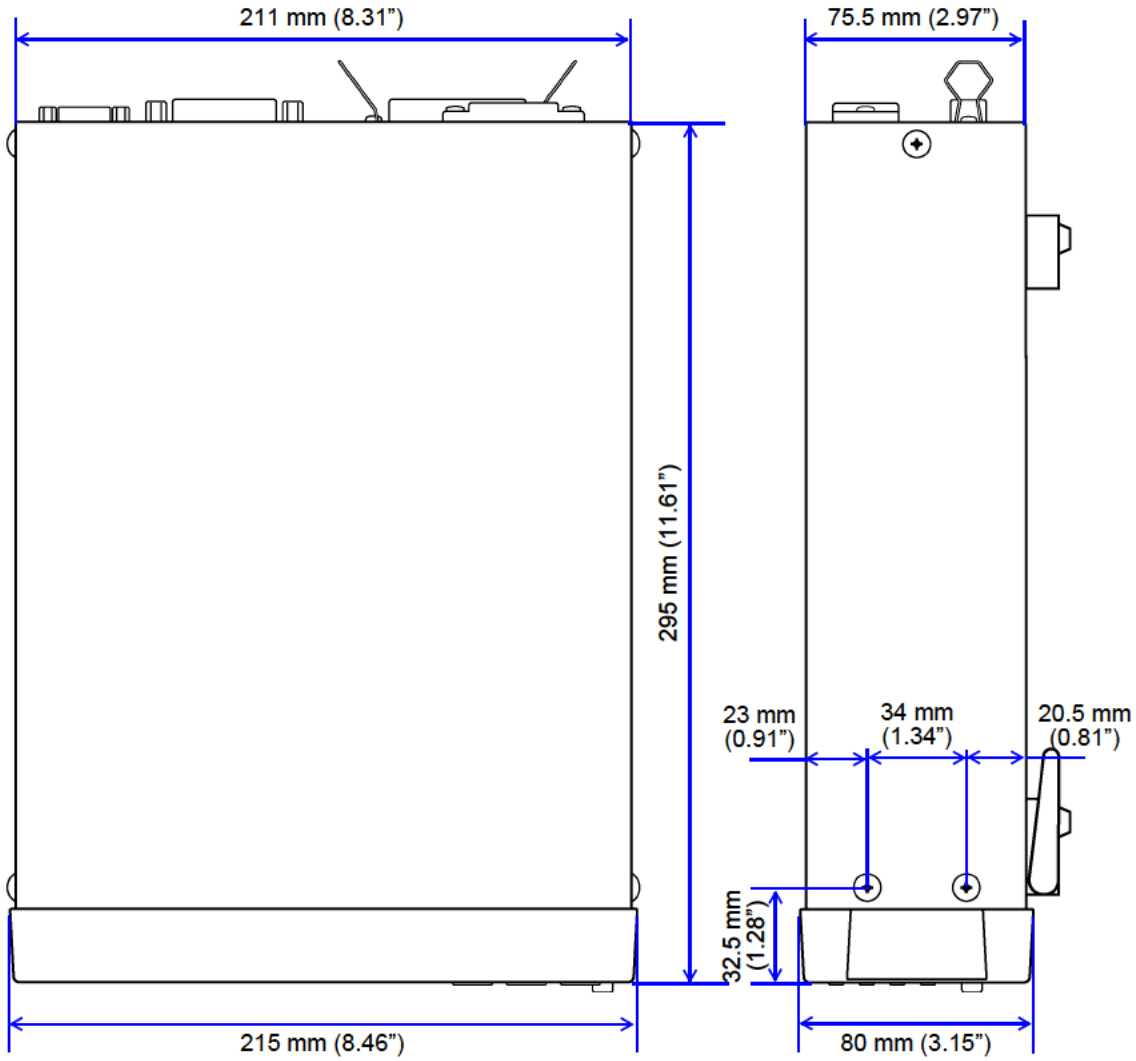

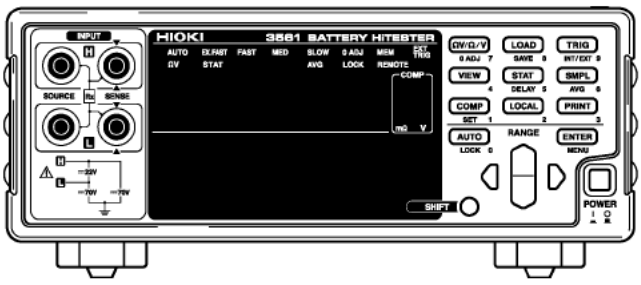

APP

Index

Numerics

0ADJ 72
3560 142
σn 47, 54
σn-1 54

A

AC four-terminal method 167
Accuracy 161
After warm-up 63
AND 49, 72
Auto-Ranging 11, 27
Averaging 11, 53

B

Before connecting and powering on 6

C

CAL 63, 71
Calibration 171
Character data 95
Cleaning 164
Clearing statistical calculation results 55
Command 92
Command compatibility 142
Comparator 11, 48
Comparator execution mode 44
Comparator function 34
Comparator judgment beeper 43
Comparator judgment results 49
Compare 34
Connector 69, 70, 89
Continuous measurement 135
CR 94
CR+LF 94
Crossover cable 90
Custom test lead 165

D

Damage 163
Data Format 95
Decimal numeric data 95
Device-Specific command 105
dgt. 3
Displayed value 27

E

EOC 72, 74, 76
EOI 94
ERR 72
Error 164
EXT I/O 12, 70
External control 69
External control terminal 77
External output terminal 78
External trigger 51, 75

F

Factory defaults 66
Footswitch 64
Format 141
Fuse 163

G

GP-IB 12, 87
Ground 6, 16, 69
Guaranteed accuracy condition 161

H

Header 93

I

IN 72
INDEX 72
Initialize 66
Input buffer 97
Input impedance 157
Input terminal 9
Inspection 21
Interface 84, 91
Internal circuitry 77
Internal trigger 51, 75
Interval printing 84, 85
Inverse-Logic output 78

J

Judge 34
Judgment results 72

K

Key beeper 65
Key-Lock 11, 60

L

LED connection 78
LF 94
Line frequency 16, 20
LOAD 62, 71
Local 102, 103, 132
LOCAL key 102

M

Main display 9, 10
MANU 72
Manual range 11
Maximum input voltage 157
Maximum rated voltage to earth 157
Mean 54
Measured current 27, 161
Measurement Fault 141
Measurement fault 32, 49, 72, 73, 74, 145, 157
Measurement mode 11, 25
measurement precision 63
Measurement range 26
Measurement setting state 61
Measurement settings 62
Measurement time 76
Measurement value output 64
Memory function 58, 128
Menu display 13

N

Noise 4, 6, 132, 163, 166
NR1 95
NR2 95
NR3 95

O

OF 32, 157
Operating key 9, 11, 65
Option 1, 172
OUT 72
Output queue 97
Overflow 32, 157

P

Panel load function 62
Panel save function 61
Period of guaranteed accuracy 162
Photocoupler connection 77, 78
Power cord 16, 21
Power inlet 12
POWER switch 9
PRINT 72
Printer 11, 79
Printing statistical calculation results 85
Process capability index 54

Q

Query 92

R

Rack mounting 173
Range 11
rdg. 3
Recording paper 82
Reference value and tolerance 45, 46
Relative value 45
Relay connection 77, 78
Remote 11, 60, 102, 103, 132
Repair 163
Reset 163
Reset function 66
Resistance and voltage measurement 25
Resistance measurement 25
Response time 158
RS-232C 12, 87

S

Sample program 147
Sampling 63
Sampling rate 11, 28
Sampling time 158
Self calibration 63, 161
SENSE-H 9, 165
SENSE-L 9, 165
Separator 94
SOURCE-H 9, 165
SOURCE-L 9, 165
Stand 12
Standard command 104, 111
Standard deviation of population 54
Statistical calculation 11
Statistical calculation function 54
Sub display 9, 10
Supply frequency 162
Supply voltage 6, 19, 162
Switch connection 77
Switching 50
Switching between measurement value and comparator setting displays 50

T

Temperature coefficient 161
Terminator 94
Test lead 17, 21, 28, 172
Threshold method 45
Timing chart 75
TRIG 51, 56, 58, 64, 71
Trigger 11, 51, 135
Trigger delay 11, 52
Trigger source 135

U

Upper and lower thresholds 45, 46

V

Voltage measurement 25

W

Warm-up time 161

Z

Zero-Adjustment 11, 28, 30

Index

HIOKI

DECLARATION OF CONFORMITY

Manufacturer's Name:	HIOKI E.E. CORPORATION
Manufacturer's Address:	81 Koizumi, Ueda, Nagano 386-1192, Japan
Product Name:	BATTERY HiTESTER
Model Number:	3561, 3561-01
Options:	9287-10 CLIP TYPE LEAD 9452 CLIP TYPE LEAD 9453 FOUR TERMINAL LEAD 9455 PIN TYPE LEAD 9467 LARGE CLIP TYPE LEAD 9770 PIN TYPE LEAD 9771 PIN TYPE LEAD

The above mentioned products conform to the following product specifications:

Safety:	EN61010-1:2001
EMC:	EN61326:1997+A1:1998+A2:2001+A3:2003 Class A equipment Equipment intented for use in industrial location EN61000-3-2:2000 EN61000-3-3:1995+A1:2001

Supplementary Information:

The products herewith comply with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC.

HIOKI E.E. CORPORATION

15 September 2006

T. Yoshiike

Tatsuyoshi Yoshiike

President

3561A999-01

HIOKI 3561, 3561-01 BATTERY HiTESTER
Instruction Manual

Publication date: September 2006 Revised edition 1

Edited and published by HIOKI E.E. CORPORATION
Technical Support Section

All inquiries to International Sales and Marketing Department
81 Koizumi, Ueda, Nagano, 386-1192, Japan
TEL: +81-268-28-0562 / FAX: +81-268-28-0568
E-mail: os-com@hioki.co.jp
URL http://www.hioki.co.jp/

Printed in Japan 3561A981-01

- All reasonable care has been taken in the production of this manual, but if you find any points which are unclear or in error, please contact your supplier or the International Sales and Marketing Department at HIOKI headquarters.
- In the interests of product development, the contents of this manual are subject to revision without prior notice.
- Unauthorized reproduction or copying of this manual is prohibited.

HIOKI

HIOKI E. E. CORPORATION

HEAD OFFICE
81 Koizumi, Ueda, Nagano 386-1192, Japan
TEL +81-268-28-0562 / FAX +81-268-28-0568
E-mail: os-com@hioki.co.jp / URL http://www.hioki.co.jp/

HIOKI USA CORPORATION
6 Corporate Drive, Cranbury, NJ 08512, USA
TEL +1-609-409-9109 / FAX +1-609-409-9108

3561A981-01 06-09H

Printed on recycled paper